



NAT'L INST. OF STAND & TECH  
A11106 360694

# NBS SPECIAL PUBLICATION 260-49

U.S. DEPARTMENT OF COMMERCE / National Bureau of Standards

*Standard Reference Materials:*

**Calibrated Glass Standards  
for Fission Track Use**

QC  
100  
.457  
no. 260-49  
1974  
c.2

## NATIONAL BUREAU OF STANDARDS

The National Bureau of Standards<sup>1</sup> was established by an act of Congress March 3, 1901. The Bureau's overall goal is to strengthen and advance the Nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research and provides: (1) a basis for the Nation's physical measurement system, (2) scientific and technological services for industry and government, (3) a technical basis for equity in trade, and (4) technical services to promote public safety. The Bureau consists of the Institute for Basic Standards, the Institute for Materials Research, the Institute for Applied Technology, the Institute for Computer Sciences and Technology, and the Office for Information Programs.

**THE INSTITUTE FOR BASIC STANDARDS** provides the central basis within the United States of a complete and consistent system of physical measurement; coordinates that system with measurement systems of other nations; and furnishes essential services leading to accurate and uniform physical measurements throughout the Nation's scientific community, industry, and commerce. The Institute consists of a Center for Radiation Research, an Office of Measurement Services and the following divisions:

Applied Mathematics — Electricity — Mechanics — Heat — Optical Physics — Nuclear Sciences<sup>2</sup> — Applied Radiation<sup>2</sup> — Quantum Electronics<sup>3</sup> — Electromagnetics<sup>3</sup> — Time and Frequency<sup>3</sup> — Laboratory Astrophysics<sup>3</sup> — Cryogenics<sup>3</sup>.

**THE INSTITUTE FOR MATERIALS RESEARCH** conducts materials research leading to improved methods of measurement, standards, and data on the properties of well-characterized materials needed by industry, commerce, educational institutions, and Government; provides advisory and research services to other Government agencies; and develops, produces, and distributes standard reference materials. The Institute consists of the Office of Standard Reference Materials and the following divisions:

Analytical Chemistry — Polymers — Metallurgy — Inorganic Materials — Reactor Radiation — Physical Chemistry.

**THE INSTITUTE FOR APPLIED TECHNOLOGY** provides technical services to promote the use of available technology and to facilitate technological innovation in industry and Government; cooperates with public and private organizations leading to the development of technological standards (including mandatory safety standards), codes and methods of test; and provides technical advice and services to Government agencies upon request. The Institute consists of a Center for Building Technology and the following divisions and offices:

Engineering and Product Standards — Weights and Measures — Invention and Innovation — Product Evaluation Technology — Electronic Technology — Technical Analysis — Measurement Engineering — Structures, Materials, and Life Safety<sup>4</sup> — Building Environment<sup>4</sup> — Technical Evaluation and Application<sup>4</sup> — Fire Technology.

**THE INSTITUTE FOR COMPUTER SCIENCES AND TECHNOLOGY** conducts research and provides technical services designed to aid Government agencies in improving cost effectiveness in the conduct of their programs through the selection, acquisition, and effective utilization of automatic data processing equipment; and serves as the principal focus within the executive branch for the development of Federal standards for automatic data processing equipment, techniques, and computer languages. The Institute consists of the following divisions:

Computer Services — Systems and Software — Computer Systems Engineering — Information Technology.

**THE OFFICE FOR INFORMATION PROGRAMS** promotes optimum dissemination and accessibility of scientific information generated within NBS and other agencies of the Federal Government; promotes the development of the National Standard Reference Data System and a system of information analysis centers dealing with the broader aspects of the National Measurement System; provides appropriate services to ensure that the NBS staff has optimum accessibility to the scientific information of the world. The Office consists of the following organizational units:

Office of Standard Reference Data — Office of Information Activities — Office of Technical Publications — Library — Office of International Relations.

<sup>1</sup> Headquarters and Laboratories at Gaithersburg, Maryland, unless otherwise noted; mailing address Washington, D.C. 20234.

<sup>2</sup> Part of the Center for Radiation Research.

<sup>3</sup> Located at Boulder, Colorado 80302.

<sup>4</sup> Part of the Center for Building Technology.

23 DEC 1974

not acc.

QC100

U57

no. 260-49

1974

C. 2

*Standard Reference Materials:*  
**Calibrated Glass Standards  
for Fission Track Use**

---

B. Stephen Carpenter and  
G. Michael Reimer

Analytical Chemistry Division  
Institute for Materials Research  
U.S. National Bureau of Standards  
Washington, D.C. 20234

*t. Special publication no. 260-49*



---

U.S. DEPARTMENT OF COMMERCE, Frederick B. Dent, Secretary  
NATIONAL BUREAU OF STANDARDS, Richard W. Roberts, Director

Issued November 1974

**Library of Congress Cataloging in Publication Data**

Carpenter, B Stephen.  
Calibrated glass standards for fission track use.

(Standard reference materials) (National Bureau of Standards  
Special Publication; 260-49)

Supt. of Docs. No.: C13.10:260-49

1. Neutron flux standards. 2. Glass—Standards. 3. Thermal  
neutrons—Measurement. I. Reimer, G. Michael, joint author. II.  
Title. III. Series: United States. National Bureau of Standards.  
Standard reference materials. IV. Series: United States. National  
Bureau of Standards. Special Publication; 260-49.

QC100.U57 No. 260-49 [QC793.5.N4626] 389'.08s 74-20566  
{539.7'62}

**National Bureau of Standards Special Publication 260-49**

Nat. Bur. Stand. (U.S.), Spec. Publ. 260-49, 27 pages (Nov. 1974)

CODEN: XNBSAV

U.S. GOVERNMENT PRINTING OFFICE  
WASHINGTON: 1974

## PREFACE

Standard Reference Materials (SRM's) as defined by the National Bureau of Standards are "well-characterized materials, produced in quantity, that calibrate a measurement system to assure compatibility of measurement in the nation." SRM's are widely used as primary standards in many diverse fields in science, industry, and technology, both within the United States and throughout the world. In many industries traceability of their quality control process to the national measurement system is carried out through the mechanism and use of SRM's. For many of the nation's scientists and technologists it is therefore of more than passing interest to know the details of the measurements made at NBS in arriving at the certified values of the SRM's produced. An NBS series of papers, of which this publication is a member, called the NBS Special Publication - 260 Series is reserved for this purpose.

This 260 Series is dedicated to the dissemination of information on all phases of the preparation, measurement, and certification of NBS-SRM's. In general, much more detail will be found in these papers than is generally allowed, or desirable, in scientific journal articles. This enables the user to assess the validity and accuracy of the measurement processes employed, to judge the statistical analysis, and to learn details of techniques and methods utilized for work entailing the greatest care and accuracy. It is also hoped that these papers will provide sufficient additional information not found on the certificate so that new applications in diverse fields not foreseen at the time the SRM was originally issued will be sought and found.

Inquiries concerning the technical content of this paper should be directed to the author(s). Other questions concerned with the availability, delivery, price, and so forth will receive prompt attention from:

Office of Standard Reference Materials  
National Bureau of Standards  
Washington, D.C. 20234

J. Paul Cali, Chief  
Office of Standard Reference Materials



## CONTENTS

	PAGE
I. INTRODUCTION . . . . .	1
II. CHARACTERIZATION OF THE GLASS STANDARDS . . . . .	2
III. CERTIFICATION AND PACKAGE DESCRIPTION . . . . .	3
IV. PREPARATION AND IRRADIATION PROCEDURES. . . . .	3
V. FLUX DETERMINATION . . . . .	4
VI. RECOMMENDED USE OF STANDARD REFERENCE MATERIALS . . . . .	6
VII. ACKNOWLEDGEMENT . . . . .	8

## LIST OF TABLES

### Table No.

I. The Uranium Concentration $^{235}\text{U}$ Isotopic Abundance . . . . .	9
II. Concentration of Elements That May Cause Track Interferences. . . . .	9
III. Activation Energies for Track Fading in the NBS Standard Glasses . . . . .	10
IV. SRM 961 Fission Track Glass Standard . . . . .	10
V. SRM 962 Fission Track Glass Standard . . . . .	11
VI. SRM 963 Fission Track Glass Standard . . . . .	12
VII. SRM 964 Fission Track Glass Standard . . . . .	13

# LIST OF FIGURES

	PAGE
Figure I. Annealing studies of uranium fission tracks in the 50 ppm SRM 962. Extrapolation of the data on this Arrhenius plot indicates that glasses used as track references should be stored in a cool place in order to prevent partial annealing of tracks . . . . .	14
Figure II. Position of RT-3 and RT-4 irradiated glasses and the four unirradiated glasses (UG) within SRM package . . . . .	15
Figure III. Arrangement of the glass, metal foils and detectors during neutron irradiation . . . . .	16



## OTHER NBS PUBLICATIONS IN THIS SERIES

- NBS Spec. Publ. 260, Standard Reference Materials: 1973 Catalog, April 1973, \$1.25.\*
- NBS Misc. Publ. 260-1, Standard Reference Materials: Preparation of NBS White Cast Iron Spectrochemical Standards, June 1964. COM 74-11061.\*\*
- NBS Misc. Publ. 260-2, Standard Reference Materials: Preparation of NBS Copper-Base Spectrochemical Standards, October 1964. COM 74-11063.\*\*
- NBS Misc. Publ. 260-3, Standard Reference Materials: Metallographic Characterization of an NBS Spectrometric Low-Alloy Steel Standard, October 1964. COM 74-11060.\*\*
- NBS Misc. Publ. 260-4, Standard Reference Materials: Sources of Information on Standard Reference Materials, February 1965. COM 74-11059.\*\*
- NBS Misc. Publ. 260-5, Standard Reference Materials: Accuracy of Solution X-Ray Spectrometric Analysis of Copper-Base Alloys, March 1965. 25 cents. (Out of print).
- NBS Misc. Publ. 260-6, Standard Reference Materials: Methods for the Chemical Analysis of White Cast Iron Standards, July 1965. COM 74-11068.\*\*
- NBS Misc. Publ. 260-7, Standard Reference Materials: Methods for the Chemical Analysis of NBS Copper-Base Spectrochemical Standards, October 1965. COM 74-11067.\*\*
- NBS Misc. Publ. 260-8, Standard Reference Materials: Analysis of Uranium Concentrates at the National Bureau of Standards, December 1965. COM 74-11066.\*\*
- NBS Misc. Publ. 260-9, Standard Reference Materials: Half Lives of Materials Used in the Preparation of Standard Reference Materials of Nineteen Radioactive Nuclides Issued by the National Bureau of Standards, November 1965. COM 74-11065.\*\*
- NBS Misc. Publ. 260-10, Standard Reference Materials: Homogeneity Characterization on NBS Spectrometric Standards II: Cartridge Brass and Low-Alloy Steel, December 1965. COM 74-11064.\*\*
- NBS Misc. Publ. 260-11, Standard Reference Materials: Viscosity of a Standard Lead-Silica Glass, November 1966. NBS Misc. Publ. 260-10.\*\*
- NBS Misc. Publ. 260-12, Standard Reference Materials: Homogeneity Characterization of NBS Spectrometric Standards III: White Cast Iron and Stainless Steel Powder Compact, September 1966. NBS Misc. Publ. 260-12.\*\*
- NBS Misc. Publ. 260-13, Standard Reference Materials: Mossbauer Spectroscopy Standard for the Chemical Shift of Iron Compounds, July 1967. NBS Misc. Publ. 260-13.\*\*
- NBS Misc. Publ. 260-14, Standard Reference Materials: Determination of Oxygen in Ferrous Materials - SRM 1090, 1091, and 1092, September 1966. NBS Misc. Publ. 260-14.\*\*
- NBS Misc. Publ. 260-15, Standard Reference Materials: Recommended Method of Use of Standard Light-Sensitive Paper for Calibrating Carbon Arcs Used in Testing Textiles for Colorfastness to Light, June 1967. NBS Misc. Publ. 260-15.\*\*
- NBS Spec. Publ. 260-16, Standard Reference Materials: Homogeneity Characterization of NBS Spectrometric Standards IV: Preparation and Microprobe Characterization of W-20% Mo Alloy Fabricated by Powder Metallurgical Methods, January 1969. COM 74-11062.\*\*
- NBS Spec. Publ. 260-17, Standard Reference Materials: Boric Acid; Isotopic and Assay Standard Reference Materials, February 1970. 65 cents.\*
- NBS Spec. Publ. 260-18, Standard Reference Materials: Calibration of NBS Secondary Standard Magnetic Tape (Computer Amplitude Reference) Using the Reference Tape Amplitude Measurement "Process A", November 1969. NBS Spec. Publ. 260-18.\*\*
- NBS Spec. Publ. 260-19, Standard Reference Materials: Analysis of Interlaboratory Measurements on the Vapor Pressure of Gold (Certification of Standard Reference Material 745), January 1970. PB 190071.\*\*
- NBS Spec. Publ. 260-21, Standard Reference Materials: Analysis of Interlaboratory Measurements on the Vapor Pressures of Cadmium and Silver, January 1971. COM 74-11359.\*\*
- NBS Spec. Publ. 260-22, Standard Reference Materials: Homogeneity Characterization of Fe-3Si Alloy, February 1971. COM 74-11357\*\*

- NBS Spec. Publ. 260-23, Standard Reference Materials: Viscosity of a Standard Borosilicate Glass, December 1970. 25 cents.\*
- NBS Spec. Publ. 260-24, Standard Reference Materials: Comparison of Redox Standards, January 1972. \$1.\*
- NBS Spec. Publ. 260-25, Standard Reference Materials: A standard Reference Material Containing Nominally Four Percent Austenite, February 1971. COM 74-11356\*\*
- NBS Spec. Publ. 260-26, Standard Reference Materials: National Bureau of Standards-U.S. Steel Corporation Joint Program for Determining Oxygen and Nitrogen in Steel, February 1971. 50 cents.\*
- NBS Spec. Publ. 260-27, Standard Reference Materials: Uranium Isotopic Standard Reference Materials, April 1971. COM 74-11358\*\*
- NBS Spec. Publ. 260-28, Standard Reference Materials: Preparation and Evaluation of SRM's 481 and 482 Gold-Silver and Gold-Copper Alloys for Microanalysis, August 1971. COM 71-50365.\*\*
- NBS Spec. Publ. 260-29, Standard Reference Materials: Calibration of NBS Secondary Standard Magnetic Tape (Computer Amplitude Reference) Using the Reference Tape Amplitude Measurement "Process A-Model 2", June 1971. COM 71-50282.\*\*
- NBS Spec. Publ. 260-30, Standard Reference Materials: Standard Samples Issued in the USSR (A Translation from the Russian), June 1971. COM 71-50283.\*\*
- NBS Spec. Publ. 260-31, Standard Reference Materials: Thermal Conductivity of Electrolytic Iron SRM 734 from 4 to 300 K, November 1971. COM 71-50563.\*\*
- NBS Spec. Publ. 260-32, Standard Reference Materials: Standard Quartz Cuvettes For High Accuracy Spectrophotometry. December 1973. 55 cents.\*
- NBS Spec. Publ. 260-33, Standard Reference Materials: Comparison of Original and Supplemental SRM 705, Narrow Molecular Weight Distribution Polystyrene, H. L. Wagner, May 1972. COM 72-50526.\*\*
- NBS Spec. Publ. 260-34, Standard Reference Materials: Thermoelectric Voltage, April 1972. COM 72-50371.\*\*
- NBS Spec. Publ. 260-35, Standard Reference Materials: Thermal Conductivity of Austenitic Stainless Steel, SRM 735 from 5 to 280 K, April 1972. 35 cents.\*
- NBS Spec. Publ. 260-36, Standard Reference Materials: A Referee Method for the Determination of Calcium in Serum. SRM 915, May 1972. COM 72-50527.\*\*
- NBS Spec. Publ. 260-37, Standard Reference Materials: Methods of Analysis of NBS Clay Standards, June 1972. COM 72-50692.\*\*
- NBS Spec. Publ. 260-38, Standard Reference Materials: Preparation and Calibration of Standards of Spectral Specular Reflectance, May 1972. 60 cents.\*
- NBS Spec. Publ. 260-39, Standard Reference Materials: The Eddy Current Decay Method for Resistivity Characterization of High-Purity Metals, May 1972. 55 cents.\*
- NBS Spec. Publ. 260-40, Standard Reference Materials: Selection of Thermal Analysis Temperature Standards Through a Cooperative Study (SRM 758, 759, 760), August 1972. 65 cents.\*
- NBS Spec. Publ. 260-41, Standard Reference Materials: Use of Standard Light-Sensitive Paper for Calibrating Carbon Arcs used in Testing Textiles for Colorfastness to Light, August 1972. COM 72-50775.\*\*
- NBS Spec. Publ. 260-42, Standard Reference Materials: The Characterization of Linear Polyethylene, SRM 1475, September 1972. 45 cents.\*
- NBS Spec. Publ. 260-43, Standard Reference Materials: Preparation and Homogeneity Characterization of an Austenitic Iron-Chromium-Nickel Alloy, November 1972. 45 cents.\*
- NBS Spec. Publ. 260-44, Standard Reference Materials: Preparation and Use of Superconductive Fixed Point Devices, SRM 767, December 1972. 75 cents.\*
- NBS Spec. Publ. 260-45, Standard Reference Materials: Powdered Lead-Based Paint, SRM 1579, March 1973. COM 73-50226.\*\*
- NBS Spec. Publ. 260-46, Standard Reference Materials: The Role of SRM's in Measurement Systems. (In press)
- NBS Spec. Publ. 260-47, Standard Reference Materials: Electrical Resistivity of Electrolytic Iron, SRM 797, and Austenitic Stainless Steel, SRM 798, from 5 to 280K, February 1974. 55 cents.\*

NBS Spec. Publ. 260-48, Standard Reference  
Materials: Description and Use of Precision  
Thermometers for the Clinical Laboratory,  
SRM 933 and SRM 934, May 1974. 60  
cents.\*

NBS Spec. Publ. 260-49, Standard Reference  
Materials: Calibrated Glass Standards for Fis-  
sion Track Use. (In preparation)

\*Send order with remittance to: Superintendent of Documents, U.S. Government Printing Office,  
Washington, D.C. 20402. Remittance from foreign countries should include an additional one-  
fourth of the purchase price for postage.

\*\*May be ordered from: National Technical Information Services (NTIS), Springfield, Virginia  
22151.



# CALIBRATED GLASS STANDARDS FOR FISSION TRACK USE

B. Stephen Carpenter and G. Michael Reimer

Analytical Chemistry Division  
Institute for Materials Research  
National Bureau of Standards  
Washington, D.C. 20234

Four glasses of different uranium concentrations were prepared and certified by the National Bureau of Standards as standards for use as neutron monitors to aid fission track studies. These Standard Reference Materials (SRM) and their uranium concentrations are: SRM 941 (461 ppm), SRM 962 (37.4 ppm), SRM 963 (0.823 ppm), and SRM 964 (0.0721 ppm). These glass wafers were irradiated in the National Bureau of Standards Reactor and the neutron flux was monitored using copper and gold foils.

Key Words: Fission tracks; flux monitors; glass standards; Standard Reference Material; thermal neutron irradiation; uranium.

## I. INTRODUCTION

The fission track technique has become an accepted and widely used method for uranium analysis and radiometric dating in many laboratories. Therefore, the need exists for a primary standard to enable correlation of inter-laboratory results. In order to fulfill this need, the National Bureau of Standards (NBS), through the Office of Standard Reference Materials, has prepared and certified Fission Track Glass Standards SRM's 961, 962, 963, and 964† (1). Although these are not the first standards prepared for fission track work (2,3), they are the first readily available fission track standards for monitoring neutron fluxes during irradiations and for comparing track densities. Since the

† Available from Office of Standard Reference Materials,  
National Bureau of Standards, Washington, D.C. 20234.

glasses have some inadequacies which will be discussed, they are not the "ideal" standards; they are, however, the best standards available at this time.

## II. CHARACTERIZATION OF THE GLASS STANDARDS

The Fission Track Glass Standards, SRM numbers 961, 962, 963, and 964, are available at four different uranium concentration levels, 461.5 ppm, 37.38 ppm, 0.823 ppm and 0.0721 ppm, respectively. These glass wafers, 12 mm in diameter and 3-mm thick, with a nominal base composition of 72% SiO<sub>2</sub>, 12% CaO, 14% Na<sub>2</sub>O, and 2% Al<sub>2</sub>O<sub>3</sub> came from the same lot of material as the Trace Element in Glass SRM's 610 through 616 (4,5,6).

This series of SRM's has been analyzed for homogeneity and was certified for approximately half of the more than 60 trace elements present at the four concentration levels, including uranium. However, in the preparation of these glasses, the uranium used for the dopant was depleted uranium, and each concentration has a different uranium-235 isotopic abundance (as seen in Table I). In determining uranium by the fission track technique, thorium and boron are two major elements that could cause possible interference since they emit charged particles that may be recorded in many external detectors. The concentrations of these two elements are given in Table II. In the certification of these glasses, the analytical competences employed by the Analytical Chemistry Division were isotope dilution mass spectrometry, polarography, flame emission and atomic absorption spectrometry, spectrophotometry, and nuclear methods of analysis, which included both neutron activation analysis and nuclear track technique.

To further characterize these standards, the thermal stability of fission tracks in the glasses was also studied to determine the fading rate of the tracks when subjected to heat. Reimer et al (7) found that the glasses had relatively low thermal stability. Extrapolation of track fading data indicates that tracks could begin to decrease at 50 °C after a time of only several months. Figure I illustrates this extrapolation for SRM 962. Table III lists the activation energies calculated from the track fading experiments that would produce a specific degree of track reduction. It is recommended that these glasses be stored below 20 °C when not being used.

### III. CERTIFICATION AND PACKAGE DESCRIPTION

The glasses are certified for the neutron flux ( $n \cdot \text{cm}^{-2} \text{sec}^{-1}$ ), in which they were irradiated. Copper and gold foils were chosen to monitor the neutron flux since many laboratories routinely use these foils.

The SRM package contains four unirradiated glass wafers and two separately irradiated wafers. The irradiations were performed in either of two positions of the NBS Reactor, each position providing different neutron energy spectra (8,9). Each package has two numbers designating the specific irradiated glasses enclosed. Figure II illustrates the configuration of the SRM package.

### IV. PREPARATION AND IRRADIATION PROCEDURES

All of the glasses were ground flat and polished on both sides, cleaned in dilute nitric acid solution (1 part  $\text{HNO}_3$ ; 10 parts  $\text{H}_2\text{O}$ ) for 2 minutes, rinsed in distilled water, ethanol, and air dried. Each cleaned wafer was then sandwiched between two pre-cleaned numbered detectors, Lexan\*

polycarbonate and muscovite mica. The combination was placed in a polyethylene bag which was hermetically vacuum sealed to ensure intimate contact between detectors and wafers. Each package was then placed in individual irradiation rabbits.

Pre-weighed foil flux monitors of copper, 0.1270-mm thick with average weight 0.021 g, and gold, 0.0254-mm thick with average weight 0.031 g, were placed in every tenth rabbit. (See Figure III for sample configuration during irradiation.) Each glass concentration level was divided into two groups of 125 samples, and each sample was irradiated individually in one of two different pneumatic tubes of the NBS Reactor (NBSR). In the radiation positions used for this work, RT-3 has a cadmium ratio of 10.2 for gold foils and 65 for copper foils, while RT-4 has a cadmium ratio of 87 for gold and 536 for copper foils (9). The irradiation time used depended on the uranium concentration and uranium-235 isotopic abundance (see Table II). Due to the high uranium content of the 961 series of glasses, the irradiations were not performed at the usual 10 MW Reactor power but at a reduced power of 1 MW.

## V. FLUX DETERMINATION

After irradiation, the gross radioactivity was allowed to decay, and the foil flux monitors were removed from the irradiation containers while external detectors and glasses were separated. The activity of the 0.511 MeV,  $^{64}\text{Cu}$  positron was counted with a 60cc Ge(Li) solid state detector; the same procedure was followed for counting the activity of the 0.412-MeV gamma-ray of  $^{198}\text{Au}$ . Each foil was counted 2 cm from the detector. The detectors had been previously calibrated with NBS SRM's chosen from the NBS radio-activity



series; therefore, absolute peak efficiencies were determined for the various  $\gamma$ -ray energies of copper and gold. The copper foils were placed between aluminum discs 0.32-mm thick in order to ensure annihilation of all  $^{64}\text{Cu}$ , 0.511-MeV positrons close to the foil. After counting all the foils that had been irradiated in the two reactor positions, the neutron flux for each foil was determined using nuclear and physical constants. The following equations were used to calculate the thermal neutron flux:

$$\text{Activity } A = \frac{C}{\bar{E} a} \quad (1)$$

A = activity in nuclear transformations per second at  $T_0$  (Time of zero decay, i.e., end of irradiation)

C = counts per second at  $T_0$

$\bar{E}$  = absolute counter efficiency for the appropriate energy gamma-ray

a = Gamma ray intensity;  $^{64}\text{Cu}(0.511 \text{ MeV}) = 0.38$ ;  $^{198}\text{Au}(0.412 \text{ MeV}) = 0.95$  (10)

$$\phi = \frac{A}{\sigma_{\text{th}} N (1 - e^{-\lambda t})} \quad (2)$$

$\phi$  = Thermal neutron flux ( $\text{n} \cdot \text{cm}^{-2} \cdot \text{sec}^{-1}$ )

$\sigma_{\text{th}}$  = Thermal neutron cross section;  $^{63}\text{Cu} = 4.5 \times 10^{-24} \text{ cm}^2$ ,  
 $^{197}\text{Au} = 98.8 \times 10^{-24} \text{ cm}^2$

N = Total number of target nuclei

$\lambda$  = Disintegration constant of radionuclide ( $^{64}\text{Au}$  or  $^{198}\text{Au}$ ) material

t = Time duration of exposure to neutron flux

The external detectors, previously separated from the glass wafers, were chemically etched to optically reveal the fission tracks. The polycarbonate detectors were etched in a 6.5N NaOH solution for 45 minutes at a constant temperature of 50 °C, then rinsed in distilled water and air dried.

The mica detectors were etched in 48% HF for 15 minutes at 20 °C, rinsed in water, and heated to dry and to volatilize any remaining HF. The irradiated glass wafers were etched in 16% HF for 75 seconds at 20 °C, rinsed with water for 15 minutes and allowed to air dry.

After etching, both of the external detectors were counted with the aid of an image analyzing microscope under the pre-established conditions of either a minimum of at least 1,000 tracks or 50 random fields of view. The random fields of view were of an area of  $1.74 \times 10^{-4} \text{ cm}^2$  at a magnification of 480X. The same counting criteria were employed for the glasses. Counting data was also collected for each series of metal foils, the two external detectors and both sides of the glasses and a statistical evaluation was performed for trends or variations in the neutron flux.

The flux determinations for glasses SRM 961, 962, 963, and 964 are reported in Tables IV, V, VI, and VII, respectively. The neutron fluence is determined by multiplying the flux by the irradiation time. There were no obvious trends or variations outside of those imposed by counting statistics that would require rejecting any of the irradiated material. However, a systematic effect was noticed for Glasses 963 and 964 which were irradiated over several days. No such errors were indicated in Glasses 961 and 962 which were all irradiated during the same day.

## VI. RECOMMENDED USE OF STANDARD REFERENCE MATERIALS

The SRM's were prepared and certified in a manner to minimize restriction of their specific use. The selection of a reactor facility, the etching conditions, and the counting criteria are all the choice of the individual laboratory.

It is recommended that one of the non-irradiated wafers, or a portion of it, be included with the samples being irradiated. The choice of the wafer included should be based upon the total expected neutron exposure and the uranium concentration of the wafer so that the number of tracks produced will be in a range convenient for counting.

After irradiation, the wafer should be polished together with the SRM irradiated wafer to remove approximately 30 micrometers from the surface, which is greater than the fragment range, thus providing an internal surface. Low speed polishing should be used to keep heating to a minimum. Both glasses should then be etched and counted together. The unknown neutron fluence can be determined from the track densities and the known neutron exposure of the SRM irradiated wafer. The counting accuracy would be dependent on the number of tracks counted.

For future irradiations, it is not necessary to repolish and re-etch the SRM irradiated standard if the etching conditions of the newly irradiated wafer are identical to those of the previously etched SRM irradiated wafer. They need only to be counted together. It is suggested, however, that all the irradiated glasses be stored below 20 °C to reduce the chance of track annealing.

The two SRM irradiated glasses allow an additional option. There was a difference in the thermal to fast neutron ratio for the irradiation of these wafers, as indicated by the cadmium ratios for gold and copper foil. The wafer selected for the counting comparisons should most closely approximate the neutron energy conditions of the reactor used. The specific glass used as a standard should always be mentioned by its NBS-SRM number in publication.

## ACKNOWLEDGEMENT

The authors would like to thank P. D. LaFleur of the Analytical Chemistry Division and the members of the Reactor Operation Section for their help in the irradiation of the glass wafers, and to L. Hernandez, J. A. Hormuth, and R. M. Young, former members of the Activation Analysis Section, for their help in packaging and preparation of the Standards. Appreciation is also extended to J. Mandel, statistical consultant for the Institute for Materials Research, for his statistical evaluation. A special note of thanks is extended to J. Paul Cali and R. E. Michaelis of the Office of Standard Reference Materials whose encouragement and support made these Standards a reality.

Certain commercial equipment, instruments, or materials are identified in this paper in order to adequately specify the experimental procedure. In no case does such identification imply recommendation or endorsement by the National Bureau of Standards, nor does it imply that the material or equipment identified is necessarily the best available for the purpose.

Table I  
The Uranium Concentration  $^{235}\text{U}$  Isotopic  
Abundance

	<u>Total U Concentration ppm (by weight)</u>	$^{235}\text{U}$ Atom Percent	<u>Reactor Location and Irradiation Time (sec.)</u>	
SRM 961	461.5 ± 1.1	0.2376	RT-3	8
			RT-4	12
SRM 962	37.38 ± 0.08	0.2392	RT-3	8
			RT-4	12
SRM 963	0.823 ± 0.002	0.2792	RT-3	80
			RT-4	120
SRM 964	0.0721 ± 0.0013	0.616	RT-3	360
			RT-4	540

Table II  
Concentration of Elements  
That May Cause Track Interferences

	<u>Boron (ppm by weight)</u>	<u>Thorium (ppm by weight)</u>
SRM 961	351	457.2 ± 1.2
SRM 962	32	37.79 ± 0.08
SRM 963	1.3	0.748 ± 0.006
SRM 964	0.20 ± 0.002	0.0252 ± 0.0007

Table III

Activation Energies for Track Fading  
in the NBS Standard Glasses

Density Reduction $\rho/\rho_0$	SRM 964	SRM 963	SRM 962	SRM 961
0.95	0.8 eV	0.7 eV	1.2 eV	0.8 eV
0.90	1.0	0.8	1.3	1.0
0.80	1.3	0.9	1.5	1.2
0.70	1.5	1.1	1.7	1.4
0.60	1.7	1.2	1.8	1.6
0.50	1.8	1.5	2.0	1.7

Table IV

SRM 961 Fission Track Glass Standard

NBS Reactor Position	Neutron Flux Mean Value and Standard Deviation <sup>a</sup> ( $\times 10^{14} \text{ n} \cdot \text{cm}^{-2} \cdot \text{sec}^{-1}$ ) <sup>b</sup>		Tolerance Intervals <sup>c</sup>	
			(95%)	(99%)
	<u>Cu Foil</u>			
RT-4	1.31	0.028	0.06	0.09
RT-3	4.56	0.086	0.20	0.28
	<u>Au Foil</u>			
RT-4	1.46	0.042	0.09	0.13
RT-3	5.43	0.17	0.39	0.55

<sup>a</sup>Standard deviations refer to individual metal foils.

<sup>b</sup>Irradiation was performed at a power of 10 megawatts;

<sup>c</sup>A 95 percent tolerance interval is estimated to include the measurement of approximately 95 percent of all individual wafers of the population of wafers. Thus, the probability is approximately 95 percent that any individual wafer measurement will lie inside the 95 percent tolerance interval. A similar definition holds for 99 percent tolerance interval.

Table V

## SRM 962 Fission Track Glass Standard

NBS Reactor Position	Neutron Flux Mean Value and Standard Deviation <sup>a</sup> ( $\times 10^{13} \text{ n} \cdot \text{cm}^{-2} \cdot \text{sec}^{-1}$ ) <sup>b</sup>	Tolerance Intervals <sup>c</sup>	
		(95%)	(99%)
<u>Cu Foil</u>			
RT-4	1.29 ± 0.072	±0.16	±0.23
RT-3	5.29 ± 0.21	±0.49	±0.69
<u>Au Foil</u>			
RT-4	1.43 ± 0.012	±0.03	±0.04
RT-3	5.93 ± 0.17	±0.40	±0.57

<sup>a</sup>Standard deviations refer to individual metal foils

<sup>b</sup>Irradiation was performed at a power of 10 megawatts; 8 seconds in RT-3, or 12 seconds in RT-4.

<sup>c</sup>A 95 percent tolerance interval is estimated to include the measurement of approximately 95 percent of all individual wafers of the population of wafers. Thus, the probability is approximately 95 percent that any individual wafer measurement will lie inside the 95 percent tolerance interval. A similar definition holds for 99 percent tolerance interval.

Table VI  
SRM 963 Fission Track Glass Standard

Wafer Number Identification	NBS Reactor Position	Neutron Flux Mean Value and Standard Deviation <sup>a</sup> ( $\times 10^{13} \text{ n} \cdot \text{cm}^{-2} \cdot \text{sec}^{-1}$ ) <sup>b</sup>	Tolerance Intervals <sup>c</sup>	
			(95%)	(99%)
<u>Cu Foil</u>				
614001-614040	RT-4	1.26 ± 0.026	±0.06	±0.09
614041-614090	RT-4	1.24 ± 0.026	±0.06	±0.09
614091-614125	RT-4	1.26 ± 0.026	±0.06	±0.09
614126-614165	RT-3	5.38 ± 0.17	±0.42	±0.60
614166-614215	RT-3	5.10 ± 0.17	±0.42	±0.59
614216-614251	RT-3	5.14 ± 0.17	±0.42	±0.60
<u>Au Foil</u>				
614001-614040	RT-4	1.41 ± 0.024	±0.06	±0.09
614041-614090	RT-4	1.36 ± 0.024	±0.06	±0.08
614091-614125	RT-4	1.44 ± 0.024	±0.06	±0.09
614126-614165	RT-3	6.03 ± 0.059	±0.15	±0.21
614166-614215	RT-3	5.97 ± 0.059	±0.15	±0.21
614216-614251	RT-3	6.13 ± 0.059	±0.15	±0.21

<sup>a</sup>Standard deviations refer to individual metal foils.

<sup>b</sup>Irradiation was performed at a power of 10 megawatts;  
80 seconds in RT-3, or 120 seconds in RT-4.

<sup>c</sup>A 95 percent tolerance interval is estimated to include the measurement of approximately 95 percent of all individual wafers of the population of wafers. Thus, the probability is approximately 95 percent that any individual wafer measurement will lie inside the 95 percent tolerance interval. A similar definition holds for 99 percent tolerance interval.



Table VII  
SRM 964 Fission Track Glass Standards

Wafer Number Identification	NBS Reactor Position	Neutron Flux Mean Value and Standard Deviation <sup>a</sup> ( $\times 10^{12} \text{n} \cdot \text{cm}^{-2} \cdot \text{sec}^{-1}$ ) <sup>b</sup>	Tolerance Intervals <sup>c</sup>	
			(95%)	(99%)
<u>Cu Foil</u>				
616001-616027	RT-4	1.31 ± 0.057	±0.15	±0.21
616028-616060	RT-4	1.26 ± 0.057	±0.15	±0.21
616061-616090	RT-4	1.32 ± 0.033	±0.08	±0.12
616091-616125	RT-4	1.39 ± 0.033	±0.08	±0.12
616126-616163	RT-3	4.84 ± 0.20	±0.52	±0.76
616164-616185	RT-3	4.57 ± 0.20	±0.57	±0.84
616186-616195	RT-3	4.50 ± 0.20	±0.66	±0.96
616196-616215	RT-3	4.55 ± 0.20	±0.57	±0.84
616216-616250	RT-3	4.41 ± 0.20	±0.52	±0.76
<u>Au Foil</u>				
616001-616027	RT-4	1.46 ± 0.033	±0.08	±0.12
616029-616060	RT-4	1.48 ± 0.033	±0.08	±0.12
616061-616090	RT-4	1.40 ± 0.057	±0.15	±0.21
616091-616125	RT-4	1.41 ± 0.057	±0.14	±0.21
616126-616163	RT-3	4.69 ± 0.10	±0.26	±0.37
616164-616185	RT-3	5.21 ± 0.10	±0.28	±0.41
616186-616195	RT-3	5.45 ± 0.10	±0.32	±0.47
616196-616215	RT-3	4.11 ± 0.10	±0.28	±0.41
616216-616250	RT-3	4.50 ± 0.10	±0.26	±0.37

<sup>a</sup>Standard deviations refer to individual metal foils.

<sup>b</sup>Irradiation was performed at a power of 10 megawatts; 360 seconds in RT-3, or 540 seconds in RT-4.

<sup>c</sup>A 95 percent tolerance interval is estimated to include the measurement of approximately 95 percent of all individual wafers of the population of wafers. Thus, the probability is approximately 95 percent that any individual wafer measurement will lie inside the 95 percent tolerance interval. A similar definition holds for 99 percent tolerance interval.

Figure I. Annealing studies of uranium fission tracks in the 50 ppm SRM 962.

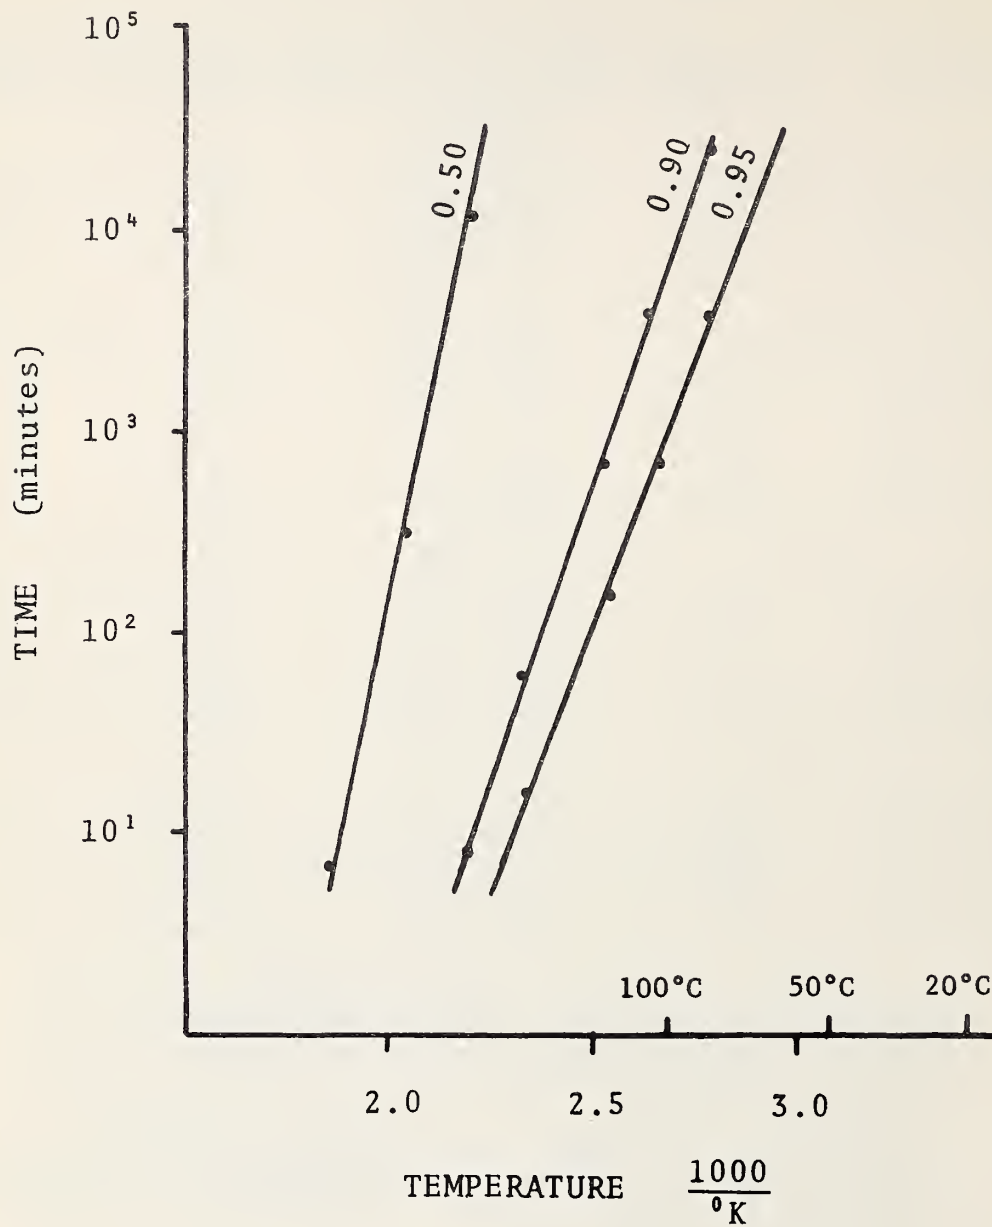


Figure II. Position of RT-3 and RT-4 irradiated glasses.


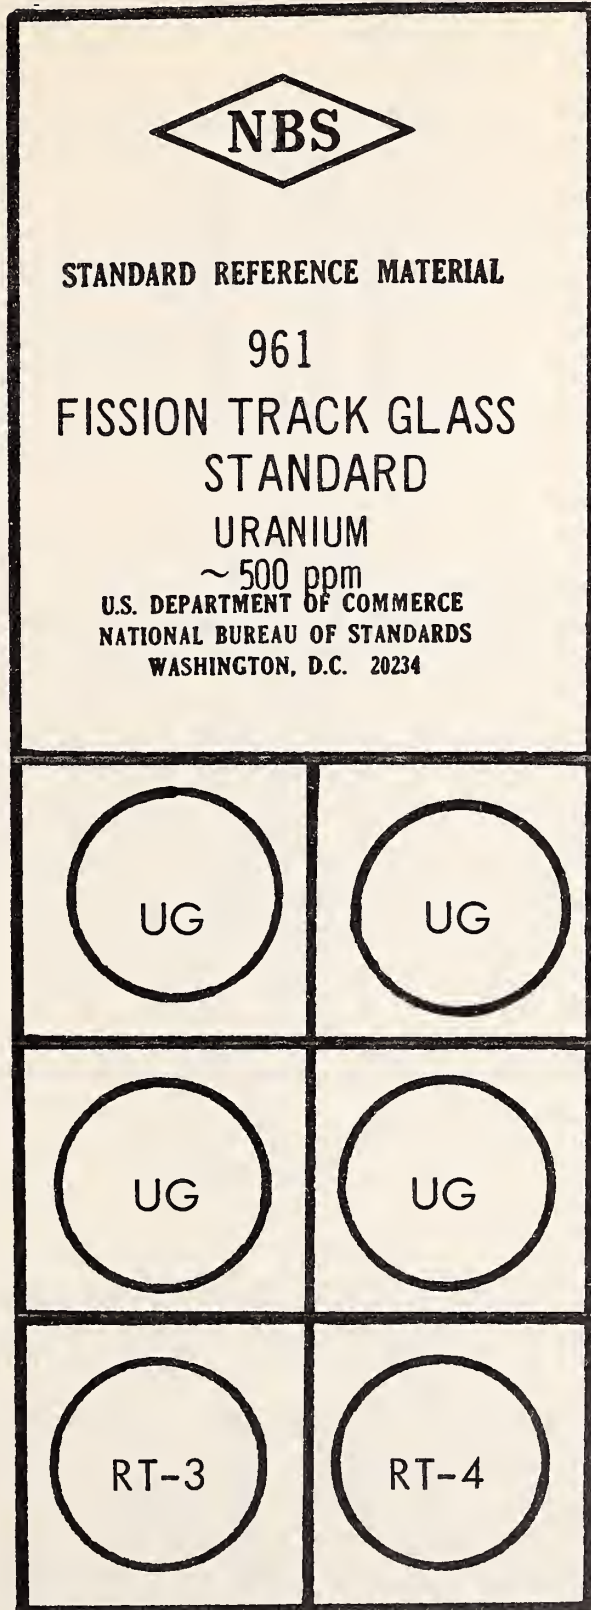


Figure III. Arrangement of the glass, metal foils and detectors during neutro irradiation.



U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. SP 260-49	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE STANDARD REFERENCE MATERIALS: Calibrated Glass Standards for Fission Track Use		5. Publication Date November 1974	
7. AUTHOR(S) B. S. Carpenter and G. M. Reimer		6. Performing Organization Code	
9. PERFORMING ORGANIZATION NAME AND ADDRESS  NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		8. Performing Organ. Report No.	
12. Sponsoring Organization Name and Complete Address (Street, City, State, ZIP)  Same as #9.		10. Project/Task/Work Unit No.	
15. SUPPLEMENTARY NOTES  Library of Congress Catalog Card Number: 74-20566		11. Contract/Grant No.	
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.)  Four glasses of different uranium concentrations were prepared and certified by the National Bureau of Standards as standards for use as neutron monitors to aid fission track studies. These Standard Reference Materials (SRM) and their uranium concentrations are: SRM 941 (461 ppm), SRM 962 (37.4 ppm), SRM 963 (0.823 ppm), and SRM 964 (0.0721 ppm). These glass wafers were irradiated in the National Bureau of Standards Reactor and the neutron flux was monitored using copper and gold foils.		13. Type of Report & Period Covered Final	
17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons) Fission tracks; flux monitors; glass standards; Standard Reference Material; thermal neutron irradiation; uranium.		14. Sponsoring Agency Code	
18. AVAILABILITY <input checked="" type="checkbox"/> Unlimited  <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS  <input checked="" type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office Washington, D.C. 20402, SD Cat. No. C13-10:260-49  <input type="checkbox"/> Order From National Technical Information Service (NTIS) Springfield, Virginia 22151	19. SECURITY CLASS (THIS REPORT) UNCLASSIFIED  UNCLASSIFIED	21. NO. OF PAGES  27	
20. SECURITY CLASS (THIS PAGE) UNCLASSIFIED  UNCLASSIFIED		22. Price  .75¢	



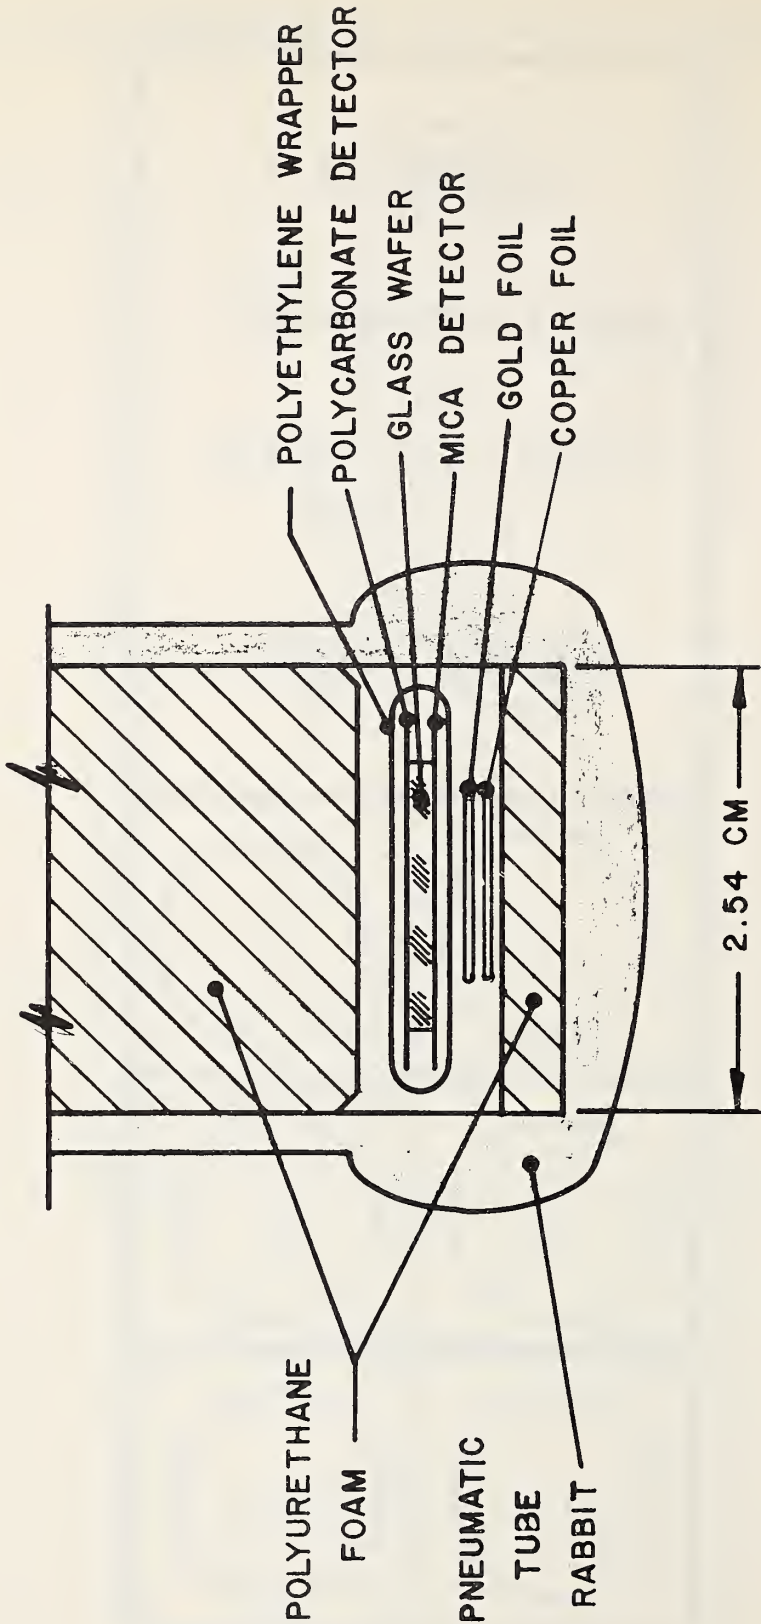

**U.S. DEPARTMENT OF COMMERCE**  
**National Bureau of Standards**  
Washington, D.C. 20234

OFFICIAL BUSINESS

Penalty for Private Use, \$300

POSTAGE AND FEES PAID  
U.S. DEPARTMENT OF COMMERCE  
COM-215

