

NBSIR 78-1350



TECHNICAL ASSOCIATION OF THE  
PULP AND PAPER INDUSTRY

COLLABORATIVE REFERENCE PROGRAM  
FOR PAPER

REPORT NO. 54G



U.S. DEPARTMENT OF COMMERCE  
National Bureau of Standards

## NBS COLLABORATIVE REFERENCE PROGRAMS

### TAPPI Paper and Board (6 times per year)

Bursting strength	Smoothness
Tearing strength	Surface pick strength
Tensile breaking strength	K & N ink absorption
Elongation to break	pH
Tensile energy absorption	Opacity
Folding endurance	Blue reflectance (brightness)
Stiffness	Specular gloss, 75°
Air resistance	Thickness
Grammage	Concora (flat crush)
	Ring crush

### FKBG-API Containerboard (48 times per year)

Mullen burst of linerboard  
Concora test of medium

### MCCA Color and Appearance (4 times per year)

Gloss at 60°  
Color and color difference  
Retroreflectivity

### Rubber (4 times per year)

Tensile strength, ultimate elongation and tensile stress  
Hardness  
Mooney viscosity  
Vulcanization properties

### ASTM Textiles (3 times per year)

Flammability (FF3-71 and FF5-74)

### ASTM Cement (2 times per year)

Chemical (11 chemical components)  
Physical (8 characteristics)

### AASHTO Bituminous

Asphalt cement (2 times per year)  
Cutbacks (once a year)



Collaborative Reference Programs  
B360 Polymer Building  
National Bureau of Standards  
Washington, D.C. 20234

TECHNICAL ASSOCIATION OF THE  
PULP AND PAPER INDUSTRY

COLLABORATIVE REFERENCE PROGRAM  
FOR PAPER

Report No. 54G

R. G. Powell  
TAPPI-NBS Research Associate  
Collaborative Testing Services, Inc.

E. B. Randall, Jr., J. Horlick  
Office of Testing Laboratory Evaluation Technology  
Office of Engineering Standards  
National Engineering Laboratory

NBSIR 78-1350

U. S. DEPARTMENT OF COMMERCE  
National Bureau of Standards



## INTRODUCTION

Reports 54S and 54G comprise the last set of reports for the 77-78 program year. Participants in tests which involve strength properties of paper will receive only the S report; those in tests which measure other properties will receive only the G report.

---

Please note that some changes have been made in the computer-generated plots. These changes should aid participants in familiarizing themselves with the International System of Units (SI) as it applies to TAPPI test methods. Wherever possible, Grand Means in SI units have been added at the top of the plots, and scales in SI units have been added to the axes allowing the reader to compare means and variability in common units and SI units for the same data. On all plots, sample codes and unit of test have been shifted to new positions.

---

Notes and comments for individual laboratories and "Best Values" applicable to a particular method are given following Table 1 for each method. See page 4 of this report for an explanation of "Best Values". Please do not confuse these best values with provisional values included with the samples to detect serious discrepancies at the time of test. NBS results, identified as L502 in the optical tests are included in some of the tables.

If there are any questions on the notes, the analyses, or the reports in general, contact Robert G. Powell, Jeffrey Horlick, or Edwin B. Randall, Jr. on 301/921-2946.



Jeffrey Horlick, Administrator  
NBS-TAPPI Collaborative Reference Program  
Office of Testing Laboratory Evaluation Technology

September 22, 1978

## BACKGROUND AND PURPOSE

In 1969, the National Bureau of Standards and the Technical Association of the Pulp and Paper Industry established a collaborative reference program to provide a participating laboratory with a means to check periodically the level and uniformity of its testing in comparison with that of other laboratories.

The interchange of paper and board products and of the raw materials for these products requires agreement among raw material suppliers, paper and board producers, converters, distributors, retailers, commercial testing laboratories, user organizations and the ultimate consumer as to the meaning of test results, an agreement that cannot be achieved without accurate and precise testing. This program is designed to help assure agreement.

## HOW THE PROGRAM WORKS

Participants Select the Tests in which they wish to participate. This choice is made on joining the program, but additional tests may be added at any time. Also new participants may enter the program at any time.

Test Samples are Distributed Bimonthly; i.e. every 2 months.

Provisional Values are Provided with the Samples for one or both of the test levels, depending on method. The provisional values permit serious discrepancies to be detected without delay. (It is left to the discretion of the laboratory supervisor as to whether these values should be known to the operator.)

Each Participant Tests the Samples, following instructions provided for each test method. The full check on a single instrument should normally take no more than 30 minutes. The test results are then sent to NBS for analysis. The participant is also asked to report other information relevant to an accurate analysis, such as test conditions and the instruments used.

Industry Means, Best Values and Other Statistics are developed from the data by NBS. The best values are estimates based on a careful examination of all data, both current and past, with special attention to results obtained by the National Bureau of Standards and other recognized reference laboratories in this and other countries.

A Quick Report is Prepared for each participating laboratory reporting data on time. This report shows the industry mean values, and the deviations of the laboratory's results from these values for each test method.

A Longer Summary Report, Showing the Data from all Participants, is also prepared. In the summary report, of which this report is an example, each laboratory is identified by a code number so that the information is maintained on a confidential basis. However, instruments are identified by type so participants can compare their results with those obtained on similar instruments of different manufacture. This report includes test averages, best values and standard deviations for individual participants and for the group as a whole. A participant should be able to readily determine the level and variability of his results in comparison with those of the other laboratories.

Repeatability and Reproducibility Statements such as Contained in ASTM, TAPPI and ISO Standards are included at the end of the report. Participants can check their performance level against the precision statement given in the test method or specification.

TABLE OF CONTENTS

Analyses In This Report

=====

PAGE

i	Introduction
ii	Description of Program
iv	Metric Conversion Table
1	Key to Tables and Graphs
5	40-1 Air Resistance, Gurley Oil type
8	40-2 Air Resistance, Sheffield type
11	41-1 Air Resistance, Gurley Mercury type
13	44-1 Smoothness, Parker Printsurf
14	45-1 Smoothness, Sheffield type
19	45-2 Smoothness, Bekk type
20	47-1 Smoothness, Bendtsen type
21	56-1 K & N Ink Absorption
22	57-1 pH, Cold Extraction
23	57-2 pH, Hot Extraction
24	60-1 Opacity, White (89%) Backing
29	60-2 Opacity, Paper Backing, B & L type
30	60-3 Opacity, Paper Backing, Elrepho type
31	65-1 Blue Reflectance (Brightness), Directional
34	65-2 Blue Reflectance, Diffuse, Elrepho (Gloss Trap)
36	65-3 Blue Reflectance, Diffuse, Elrepho (No Gloss Trap)
38	75-1 Specular Gloss, 75 degree
41	90-1 Thickness (Caliper)
46	95-1 Grammage (Basis Weight)
49	Summary

Analyses In The S Report

=====

10-1	Bursting Strength = Up to 45 psi
10-2	Bursting Strength = Up to 45 psi, Air Clamps
11-1	Bursting Strength = Up to 100 psi
15-1	Tearing Strength = Deep Cutout
17-1	Tearing Strength = No Cutout
19-1	Tensile Breaking Strength = Packaging Papers
20-1	Tensile Breaking Strength = Printing Papers, CRE
20-2	Tensile Breaking Strength = Printing Papers, Pendulum
25-1	Tensile Energy Absorption = Packaging Papers
26-1	Tensile Energy Absorption = Printing Papers
28-1	Elongation to Break = Packaging Papers
29-1	Elongation to Break = Printing Papers
30-1	Folding Endurance, MIT type
30-2	Folding Endurance, MIT type, log (base 10)
35-1	Stiffness, Gurley
36-1	Stiffness, Taber
49-1	Surface Pick Strength, IGT
50-1	Surface Pick Strength, Wax
91-1	Concora (Flat Crush)
96-1	Ring Crush

TABLE OF CONVERSION FACTORS TO METRIC (SI) UNITS

<u>Physical Quantity</u>	<u>To Convert From</u>	<u>To</u>	<u>Multiply by</u>
Bursting strength	psi	kPa	6.895
	kg/cm <sup>2</sup>	kPa	98.07
	bar	kPa	100.00
Tearing strength	g	mN	9.807
Tensile strength	lb/in.	kN/m	.1751
	lb/0.5 in.	kN/m	.3502
	lb/15 mm	kN/m	.2965
	kg/15 mm	kN/m	.6538
	kg/25 mm	kN/m	.3923
	kg/mm	kN/m	9.807
Tensile energy absorption	ft-lb/ft <sup>2</sup>	J/m <sup>2</sup>	14.59
	in.-lb/in. <sup>2</sup>	J/m <sup>2</sup>	175.1
	kg-m/m <sup>2</sup>	J/m <sup>2</sup>	9.807
Bending stiffness	g·cm	μN·m	98.07
Flat-crush strength (Concora)	lb	N	4.448
Ring-crush (TAPPI) (ISO)	lb	N	4.448
	lb/6.00 in.	kN/m	0.0292
Thickness	mil	μm	25.40

## KEY TO TABLES AND GRAPHS

MEAN -	The average of individual TEST DETERMINATIONS. The number of TEST DETERMINATIONS in the mean is given in the upper right corner of the first table (TEST D.) and again at the bottom of this table.
GRAND MEAN - (GR. MEAN)	The average of the individual laboratory MEANS, excluding laboratories flagged (see column F) with an X, #, or +. The GRAND MEAN is given in US customary units and, where applicable, in SI metric units.
SD OF MEANS - (SD MEANS)	The standard deviation of the laboratory MEANS about the GRAND MEAN; an index of the among-laboratory precision.
DEV -	The deviation or difference of the laboratory MEAN from the GRAND MEAN.
N. DEV -	The normal deviate or ratio of the DEV to the SD OF MEANS; an indication of the degree of divergence of the laboratory MEAN from the GRAND MEAN. A N. DEV of more than 2 or less than -2 may indicate that the participant is not following the procedure considered standard for this analysis.
SDR -	The standard deviation of repeated measurements; that is, of individual test determinations about their MEAN.
AVERAGE SDR -	The average of the individual laboratory SDR's; an index of the within-laboratory precision of repeated measurements.
R. SDR -	The relative standard deviation of repeated measurements; that is, the ratio of the SDR to the AVERAGE SDR; an indication of the ability of a participant to repeat his measurements relative to the average ability. The greater the number of TEST DETERMINATIONS the closer the R. SDR should be to unity. If R. SDR is outside the limits given below, the participant may not be following the procedure considered standard for this analysis:

No. of test Determinations	Lower limit for R. SDR	Upper limit for R. SDR
3	0.09	2.58
5	0.27	2.06
8	0.40	1.77
10	0.46	1.67
15	0.56	1.53
20	0.61	1.45
25	0.65	1.39

VAR - Code for instrument type or variation in condition, see second table.

F - Flag, with following meaning:

+ - Excluded from grand means because VAR non-standard for this analysis.

# - Excluded because data were not understood or because of a non-coded variation reported by the laboratory. (See NOTES following Table 1 for each method).

M - Excluded because data for one sample are missing.

X - Excluded because plotted point would fall outside of the 99% error ellipse, (see below for explanation of Graph).

\* - Included in grand means but plotted point falls outside of the 95% error ellipse. The participants should take this as a warning to reexamine his testing procedure.

S - Included in grand mean but only after omission of one or more 'wild' values; that is, test determinations more than 3 times AVERAGE SDR from the laboratory's MEAN. Not more than 20% of the test determination may be excluded in this manner without rejecting the laboratory.

0 - Included in grand mean and inside 95% error ellipse.

## COORDINATES -

Distances along major and minor axes of error ellipse. If special additive or concurrent model of the measuring process applies to this method, the distance along the minor axis represents the random error within a laboratory while that along the major axis also includes a systematic laboratory component of error.

**95% ELLIPSE -**

Lengths of the major and minor axes of the ellipse and the angle that the major axis makes with the horizontal axis.

**AVG R. SDR -**

Average of the R. SDR for the two samples; an indication of the laboratory's precision of repeated measurements.

**Graph -**

For each laboratory the MEAN for the second sample is plotted against the MEAN for the first sample, with each point representing a laboratory. The horizontal and vertical lines are the GRAND MEANS. The dashed line is drawn at 45°. The solid sloping line, which may or may not lie close to the 45° line, is along the major axis of the error ellipse. The ellipse is drawn so that, on the average, it will include 95% of the points representing the laboratories.

Plotted symbols are as explained above (under F), except that an 'S' is plotted as an 'O'. A participant whose plotted point falls outside of the ellipse should carefully reexamine the testing procedure he is following.

The graph is plotted with an ellipse when there are 20 or more laboratories in the analysis. When there are 10 through 19 laboratories in the analysis the graph is plotted but the ellipse is omitted. When there are fewer than 10 laboratories retained in the analysis the graph is not plotted.

The International System of Units (SI) is used on the plots wherever possible to aid participants in familiarizing themselves with SI. Grand means in SI units are given at the top of the plot, and supplementary scales in SI units are drawn along the axes allowing the reader to compare means and variability in common units and SI units for the same data.

Summary -  
(At end of  
report)

In addition to several quantities already defined above, the summary shows the following values for each test method:

REPL CRP -

The number of replicate test determinations used in this Collaborative Reference Program.

REPL TAPPI -

The number of replicate test determinations in a test result required by the applicable TAPPI Standard or assumed here if there is no TAPPI Standard. This quantity is needed in the computation of TAPPI repeatability and reproducibility from the SD OF MEANS and the AVER SDR. See TAPPI Standard T1206 for definitions and computations.

REPEAT -

TAPPI repeatability, a measure of the within-laboratory precision of a test result.

REPROD -

TAPPI reproducibility, a measure of the between-laboratory precision of a test result.

Best values -

Given at the end of Table 1 for each method for which sufficient information is available. These best values are estimates based on a careful examination of all data, both current and past, with special attention to results obtained by the National Bureau of Standards and other recognized reference laboratories in this and other countries. All participants using equipment that is standard for the analysis should be able to achieve results within the plus-minus (+) limits, when these are shown along with the best values.

ANALYSIS T40-1 TABLE I  
 AIR RESISTANCE, GURLEY UNITS (SECONDS/100 CC)  
 TAPPI STANDARD T460 GS-75, AIR RESISTANCE OF PAPER

LAB CODE	SAMPLE J47	PRINTING					SAMPLE E73	HEAT SET OFFSET BOOK					TEST D. = 10			
		106 GRAMS PER SQUARE METER						76 GRAMS PER SQUARE METER					VAR	F	LAB	
		MEAN	DEV	N. DEV	SDR	R. SDR		MEAN	DEV	N. DEV	SDR	R. SDR				
L107	29.5	.5	.47	1.3	.87	17.6	.1	.08	1.7	1.11	40D	Ø	L107			
L121	29.7	.3	.32	1.4	.97	18.7	1.2	1.06	1.6	1.04	40D	Ø	L121			
L122	30.3	.2	.23	1.5	1.06	17.6	.1	.12	1.0	.64	40D	Ø	L122			
L123	29.6	.4	.42	1.3	.89	16.8	.7	.65	1.5	1.02	40D	Ø	L123			
L124G	27.7	-2.3	-2.17	1.6	1.10	15.8	-1.7	-1.55	1.6	1.07	40D	Ø	L124G			
L125	30.9	.8	.81	1.7	1.18	16.9	.6	.55	1.1	.75	40D	Ø	L125			
L127	29.8	.2	.20	1.4	.94	17.3	.2	.21	1.1	.75	40D	Ø	L127			
L128	30.8	.8	.73	1.5	1.01	19.5	2.0	1.78	1.1	.71	40D	Ø	L128			
L141	30.7	.7	.64	1.5	1.02	17.9	.4	.32	1.8	1.21	40D	Ø	L141			
L148	30.8	.8	.73	1.3	.88	18.7	1.1	1.03	1.7	1.13	40D	Ø	L148			
L153	29.6	.4	.41	2.2	1.48	15.6	-1.9	-1.74	1.0	.68	40D	Ø	L153			
L158	28.7	-1.3	-1.27	2.2	1.47	18.3	.8	.71	1.3	.83	40D	Ø	L158			
L159	31.3	1.3	1.22	2.6	1.74	18.3	.7	.67	1.6	1.03	40D	Ø	L159			
L163	30.7	.7	.63	1.2	.79	19.8	2.3	2.06	1.7	1.09	40D	Ø	L163			
L166	31.5	1.5	1.41	1.8	1.25	16.4	-1.1	-1.02	1.9	1.25	40D	Ø	L166			
L174	30.6	.6	.54	1.8	1.21	16.4	-1.1	-1.01	1.8	1.19	40D	Ø	L174			
L176	34.4	4.4	4.15	1.3	.86	19.6	2.1	1.90	2.3	1.54	40D	#	L176			
L182G	28.8	-1.2	-1.17	1.8	1.19	16.8	.7	.64	1.9	1.23	40D	Ø	L182G			
L190C	30.8	.8	.73	1.5	1.06	18.9	1.3	1.21	2.2	1.43	40D	Ø	L190C			
L190R	29.2	.8	.79	1.1	.77	17.3	.2	.15	1.7	1.10	40D	Ø	L190R			
L223	31.8	1.8	1.73	1.2	.83	18.3	.8	.74	.9	.60	40D	Ø	L223			
L224	29.0	-1.0	-.96	1.5	1.05	15.4	-2.1	-1.85	2.5	1.66	40D	Ø	L224			
L230G	30.7	.7	.64	1.1	.72	17.3	-.2	-.19	1.3	.83	40D	Ø	L230G			
L238A	30.5	.5	.45	2.0	1.37	17.4	.1	.10	.8	.53	40D	Ø	L238A			
L241	27.6	-2.4	-2.31	1.4	.97	16.1	-1.4	-1.26	1.4	.96	40D	Ø	L241			
L243G	28.8	-1.2	-1.17	1.1	.77	17.6	.1	.10	1.7	1.11	40D	Ø	L243G			
L259	27.4	-2.7	-2.54	2.4	1.61	18.0	.5	.43	1.6	1.08	40D	#	L259			
L261	29.7	-.3	-.31	1.8	1.20	17.0	-.5	-.43	1.0	.67	40D	Ø	L261			
L262G	29.9	-.1	-.10	1.2	.80	18.0	.5	.46	.8	.54	40D	Ø	L262G			
L265	29.8	-.3	-.26	1.3	.87	17.1	-.4	-.32	1.9	1.27	40D	Ø	L265			
L278	30.9	.8	.81	1.1	.72	17.5	.0	.03	1.8	1.17	40D	Ø	L278			
L285	31.4	1.3	1.27	1.0	.69	17.7	.2	.14	2.0	1.31	40D	Ø	L285			
L301	29.1	-.9	-.90	2.3	1.54	17.3	-.2	-.16	1.6	1.08	40D	Ø	L301			
L308	31.9	1.9	1.78	1.2	.82	18.2	.7	.64	1.4	.96	40D	Ø	L308			
L312	29.7	-.3	-.32	2.0	1.37	17.1	-.4	-.37	1.2	.79	40D	Ø	L312			
L321	30.6	.6	.54	2.7	1.82	15.2	-2.3	-2.07	2.1	1.42	40D	Ø	L321			
L324	29.2	-.8	-.76	1.4	.95	17.9	.3	.31	1.4	.96	40D	Ø	L324			
L326	30.8	.8	.73	.9	.63	18.5	1.0	.91	1.1	.72	40D	Ø	L326			
L328	30.0	-.0	-.01	.8	.52	17.5	.0	.02	.6	.40	40D	Ø	L328			
L341	31.4	1.3	1.28	1.2	.79	19.2	1.6	1.48	1.2	.78	40D	Ø	L341			
L344	29.2	-.8	-.75	1.2	.79	17.5	-.0	-.01	1.9	1.24	40D	Ø	L344			
L376	31.2	1.2	1.15	1.5	1.03	18.8	1.3	1.20	1.9	1.25	40D	Ø	L376			
L380	30.0	-.0	-.03	.8	.56	19.6	2.1	1.87	.8	.55	40D	Ø	L380			
L396M	29.1	-.9	-.84	1.5	1.02	15.1	-2.4	-2.16	1.5	1.00	40D	Ø	L396M			
L561	29.1	-.9	-.89	1.4	.93	17.4	-.1	-.10	1.4	.95	40D	Ø	L561			
L567	29.9	-.1	-.13	1.2	.82	17.2	-.3	-.28	1.4	.93	40D	Ø	L567			
L576	29.5	-.5	-.47	1.0	.68	17.7	.2	.21	1.6	1.06	40D	Ø	L576			
L599	30.0	-.0	-.01	1.4	.97	16.8	-.7	-.59	1.8	1.22	40D	Ø	L599			
L604	29.8	-.2	-.18	1.8	1.20	15.7	-1.8	-1.60	1.7	1.15	40D	Ø	L604			
L616	31.1	1.0	.98	.6	.41	17.9	.4	.34	2.4	1.61	40D	Ø	L616			
L676	31.2	1.2	1.13	1.9	1.28	18.7	1.2	1.09	1.6	1.04	40D	Ø	L676			
GR. MEAN =	30.0	GURLEY UNITS					GRAND MEAN =	17.5	GURLEY UNITS					TEST DETERMINATIONS = 10		
SD MEANS =	1.1	GURLEY UNITS					SD OF MEANS =	1.1	GURLEY UNITS					50 LABS IN GRAND MEANS		
AVERAGE SDR =	1.5	GURLEY UNITS					AVERAGE SDR =	1.5	GURLEY UNITS					TEST DETERMINATIONS = 10		
L115	27.4	-2.6	-2.50	1.2	.80	15.6	-1.9	-1.71	1.5	1.00	40U	♦	L115			
L236	30.5	.5	.49	1.5	1.01	18.2	.7	.65	1.5	1.00	40E	♦	L236			
L291	30.2	.2	.16	1.5	1.06	19.1	1.6	1.42	2.1	1.41	40U	♦	L291			
L484	28.5	-1.6	-1.48	1.0	.65	16.7	-.8	-.75	1.1	.74	40H	♦	L484			

TOTAL NUMBER OF LABORATORIES REPORTING = 55

Best values: J47 29.5  $\pm$  1.8 Gurley units  
 .B73 17.5  $\pm$  1.9 Gurley units


The following laboratories were omitted from the grand means because of extreme test results: 176

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T40-1 TABLE 2  
AIR RESISTANCE, GURLEY UNITS (SECONDS/100 CC)  
TAPPI STANDARD T460 GS-75. AIR RESISTANCE OF PAPER

JUNE 1978

LAB CODE	P	MEANS J47	COORDINATES E73	AVG MAJOR	MINOR	R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L259	*	27.4	18.0	-1.4	2.3	1.34 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L115	*	27.4	15.6	-3.2	.8	.90 40U AIR RESISTANCE, SHEFFIELD IN GURLEY UNITS	
L241	0	27.6	16.1	-2.7	.9	.97 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L124G	0	27.7	15.8	-2.8	.6	1.08 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L484	*	28.5	16.7	-1.6	.6	.70 40H AIR RESISTANCE, REGMED-TYPE GURLEY DENSOMETER - GIL FLOTATION	
L158	0	28.7	18.3	-3	1.5	1.15 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L243G	0	28.8	17.6	-7	1.0	.94 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L182G	0	28.8	16.8	-1.3	.5	1.21 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L224	0	29.0	15.4	-2.2	.6	1.35 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L301	0	29.1	17.3	-7	.6	1.31 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L561	0	29.1	17.4	-7	.6	.94 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L396W	0	29.1	15.1	-2.4	.9	1.01 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L190R	0	29.2	17.3	-7	.5	.93 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L324	0	29.2	17.9	-3	.8	.95 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L344	0	29.2	17.5	-5	.6	1.01 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L576	0	29.5	17.7	-1	.5	.87 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L107	0	29.5	17.6	-3	.4	.99 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L123	0	29.6	16.8	-8	.1	.96 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L153	0	29.6	15.6	-1.8	.9	1.08 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L121	0	29.7	18.7	.7	1.0	1.00 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L312	0	29.7	17.1	-5	0.0	1.08 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L261	0	29.7	17.0	-6	1	.94 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L265	0	29.8	17.1	-5	0.0	1.07 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L127	0	29.8	17.3	-3	0	.85 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L604	0	29.8	15.7	-1.5	-1.0	1.17 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L567	0	29.9	17.2	-3	.1	.87 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L262G	0	29.9	18.0	.3	.4	.67 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L380	0	30.0	19.6	1.6	1.4	.56 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L328	0	30.0	17.5	.0	.0	.46 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L599	0	30.0	16.8	-5	-0.4	1.09 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L291	*	30.2	19.1	1.3	.9	1.23 40U AIR RESISTANCE, SHEFFIELD IN GURLEY UNITS	
L122	0	30.3	17.6	.3	-1	.85 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L238A	0	30.5	17.4	.2	-4	.95 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L236	*	30.5	18.2	.9	.1	1.00 40E AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION, 20C, 65%RH	
L174	0	30.6	16.4	-5	-1.2	1.20 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L321	0	30.6	15.2	-1.4	-1.9	1.62 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L163	0	30.7	19.8	2.2	1.0	.94 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L2300	0	30.7	17.3	.3	-6	.78 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L141	0	30.7	17.9	.7	-3	1.11 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L148	0	30.8	18.7	1.4	.2	1.00 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L128	0	30.8	19.5	2.0	.7	.86 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L326	0	30.8	18.5	1.3	.1	.67 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L190C	0	30.8	18.9	1.5	.3	1.24 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L278	0	30.9	17.5	.6	-6	.94 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L125	0	30.9	16.9	.1	-1.0	.97 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L616	0	31.1	17.9	1.0	-5	1.01 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L676	0	31.2	18.7	1.7	-1	1.16 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L376	0	31.2	18.8	1.8	-0	1.14 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L159	0	31.3	18.3	1.4	-5	1.39 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L285	0	31.4	17.7	1.0	-9	1.00 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L341	0	31.4	19.2	2.1	0	.79 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L166	0	31.5	16.4	.1	-1.9	1.25 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L223	0	31.8	18.3	1.8	-8	.71 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L308	0	31.9	18.2	1.8	-1.0	.89 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
L176	#	34.4	19.6	4.5	-1.9	1.20 40D AIR RESISTANCE, GURLEY DENSOMETER - GIL FLOTATION	
GMEANS:		30.0	17.5		1.00		
95% ELLIPSE:		3.3	2.1		WITH GAMMA = 49 DEGREES		

# AIR RESISTANCE, GURLEY

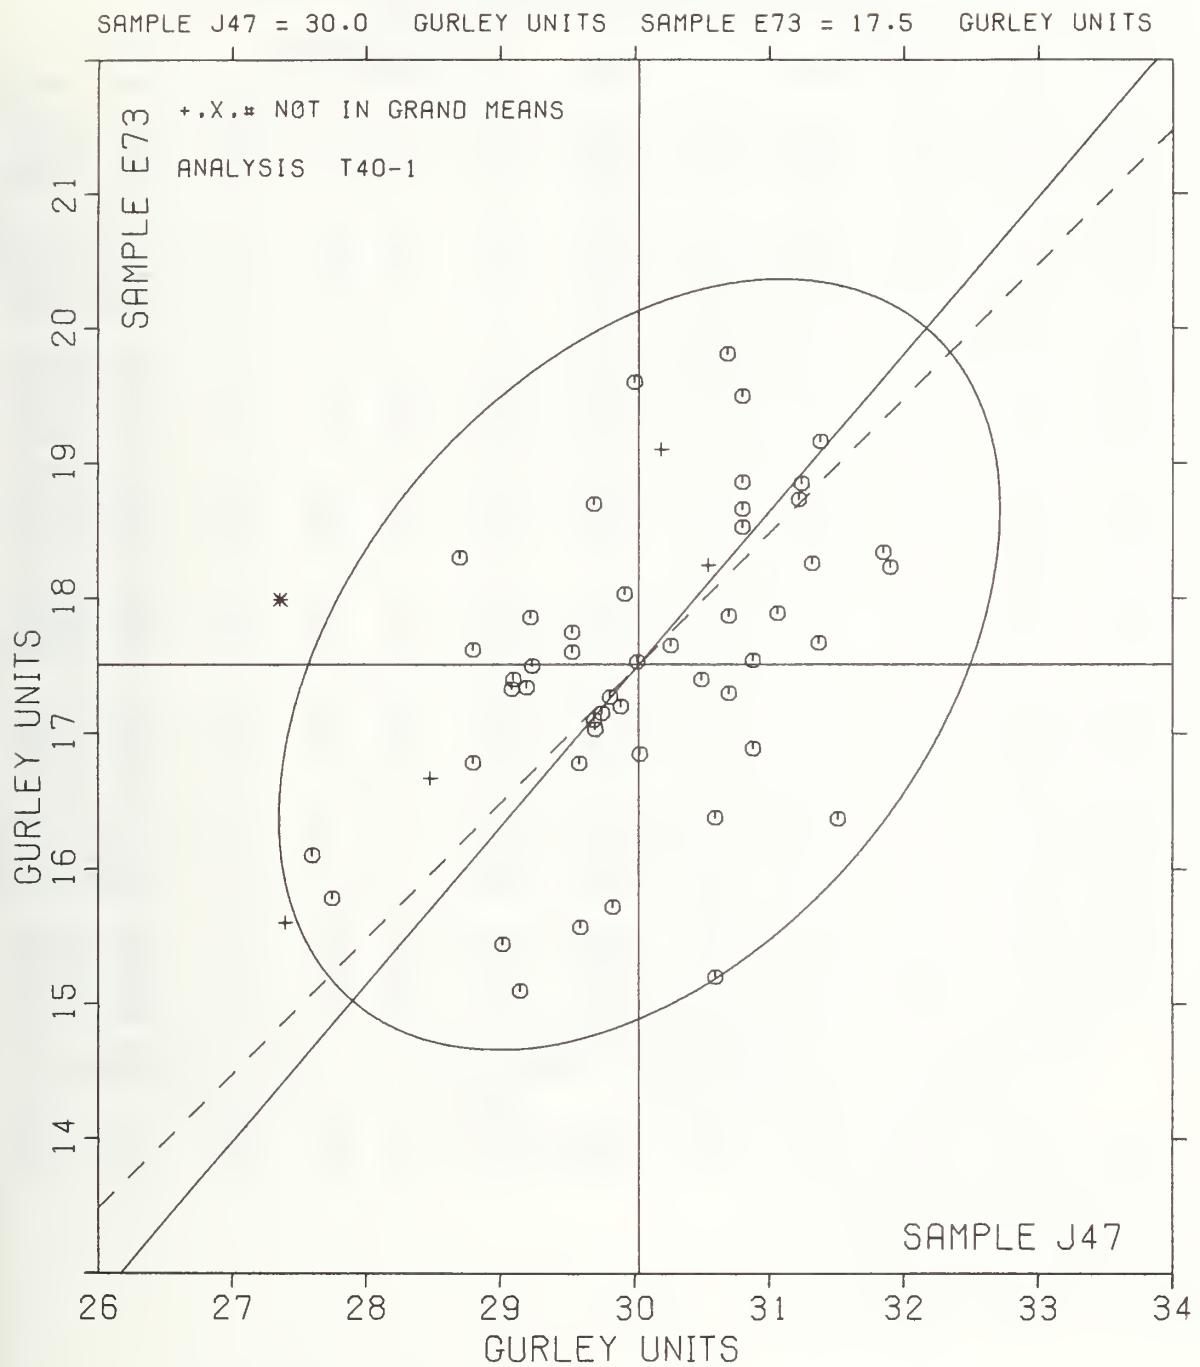

ANALYSIS T40-2 TABLE 1  
 AIR RESISTANCE. SHEFFIELD UNITS (CC/MIN) FOR 0.442 SQ. IN (3/4 IN. DIA) ORIFICE  
 SHEFFIELD TESTER IS STANDARD FOR THIS ANALYSIS

LAB CGDE	SAMPLE J47	PRINTING					SAMPLE E73	HEAT SET OFFSET BOOK					TEST D. = 10		
		106 GRAMS MEAN	DEV	N. DEV	SDR	R. SDR		76 GRAMS MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L114	110.5	4.2	.90	3.7	.92		166.8	8.9	1.25	15.2	1.38	40S	G	L114	
L121	104.3	-2.0	-0.43	4.1	1.04		160.8	2.9	.41	15.3	1.38	40S	G	L121	
L122S	109.1	2.8	.60	5.6	1.43		156.2	-1.7	-0.24	11.3	1.02	40S	G	L122S	
L124S	103.1	-3.2	-0.69	6.1	1.54		151.6	-6.3	-0.89	14.3	1.29	40S	G	L124S	
L127	108.5	2.2	.47	2.9	.74		152.2	-5.7	-0.81	8.9	.80	40S	G	L127	
L132	104.4	-1.9	-0.41	3.8	.95		158.7	.8	.11	10.2	.92	40S	G	L132	
L148	110.0	3.7	.79	3.5	.87		159.8	1.9	.26	13.9	1.25	40S	G	L148	
L157	107.4	1.1	.23	2.8	.71		152.2	-5.7	-0.81	12.1	1.09	40S	G	L157	
L158	100.0	-6.3	-1.35	3.3	.84		151.0	-6.9	-0.98	9.9	.90	40S	G	L158	
L173B	104.0	-2.3	-0.49	2.1	.53		158.0	.1	.01	11.4	1.02	40S	G	L173B	
L190C	105.3	-1.0	-0.22	4.1	1.02		156.0	-1.9	-0.27	13.9	1.26	40S	G	L190C	
L213	115.7	9.4	2.01	2.2	.55		165.8	7.9	1.11	7.8	.70	40S	G	L213	
L223	99.6	-6.7	-1.43	3.7	.92		161.6	3.7	.52	17.6	1.59	40S	G	L223	
L228	131.1	24.8	5.30	5.9	1.48		191.4	33.5	4.72	12.8	1.15	40S	#	L228	
L230S	99.7	-6.6	-1.41	3.1	.78		147.2	-10.7	-1.51	14.7	1.33	40S	G	L230S	
L233	105.6	.7	-0.15	4.6	1.16		155.0	-2.9	-0.41	9.3	.84	40S	G	L233	
L241	115.0	8.7	1.86	4.7	1.19		164.0	6.1	.86	12.2	1.10	40S	G	L241	
L249	99.6	-6.7	-1.43	3.4	.87		152.8	-5.1	-0.72	16.4	1.48	40S	G	L249	
L255	107.7	1.4	.30	3.9	1.00		161.9	4.0	.56	11.1	1.00	40S	G	L255	
L257A	110.9	4.6	.98	3.5	.89		157.5	-.4	-0.06	9.7	.88	40S	G	L257A	
L257B	108.2	1.9	.40	5.5	1.40		163.7	5.8	.81	9.8	.89	40S	G	L257B	
L257C	110.9	4.6	.98	3.3	.84		159.3	1.4	.19	7.3	.66	40S	G	L257C	
L260	109.1	2.8	.60	4.7	1.20		165.3	7.4	1.04	7.9	.72	40S	G	L260	
L262S	101.5	-4.8	-1.03	3.6	.91		140.4	-17.5	-2.47	6.6	.60	40S	G	L262S	
L288	113.8	7.5	1.60	6.4	1.61		169.4	11.5	1.62	10.2	.92	40S	G	L288	
L301	114.1	7.8	1.67	7.0	1.77		172.1	14.2	2.00	11.5	1.04	40S	G	L301	
L305	110.2	3.9	.83	3.5	.89		159.0	1.1	.15	5.2	.47	40S	G	L305	
L312	101.4	-4.9	-1.05	2.4	.61		159.8	1.9	.26	6.4	.58	40S	G	L312	
L318	101.8	-4.5	-0.96	4.7	1.18		155.8	-2.1	-0.30	11.1	1.00	40S	G	L318	
L349	101.9	-4.4	-0.94	3.9	.99		152.6	-5.3	-0.75	9.2	.83	40S	G	L349	
L352	104.7	-1.6	-0.34	3.6	.90		151.5	-6.0	-0.85	10.0	.90	40S	G	L352	
L354	109.2	2.9	.62	4.2	1.07		151.6	-6.3	-0.89	7.6	.68	40S	G	L354	
L360	105.3	-1.0	-0.22	2.5	.62		147.7	-10.2	-1.44	12.5	1.12	40S	G	L360	
L370	102.7	-3.6	-0.77	4.4	1.12		160.8	2.9	.41	8.6	.77	40S	G	L370	
L390	101.3	-5.0	-1.07	5.3	1.35		152.9	-5.0	-0.71	13.2	1.19	40S	G	L390	
L562	293.0	186.7	39.90	17.7	4.46		338.0	180.1	25.39	29.7	2.68	40S	#	L562	
L575	106.9	.6	.13	3.1	.78		169.4	11.5	1.62	15.4	1.39	40S	G	L575	
L587	109.9	3.6	.77	4.6	1.15		164.3	6.4	.90	13.4	1.21	40S	G	L587	
L597	108.0	1.7	.36	2.7	.68		167.5	9.6	1.35	13.6	1.22	40S	G	L597	
L626	98.4	-7.9	-1.69	3.8	.97		148.6	-9.3	-1.31	6.6	.60	40S	G	L626	

GR. MEAN = 106.3 SHEPP. UNITS

GRAND MEAN = 157.9 SHBFF. UNITS

**TEST DETERMINATIONS - 10**

SD MEANS = 4.7 SHEPP. UNITS  
AVERAGE

SD OF MEANS = 7.1 SHEPP. UNITS

**38 LABS IN GRAND MEANS**

**AVERAGE**

**O SHEFF. UNITS**                           **AVERAGE**

## I SHEFF. UNITS

1182B 413.6 303.3 65.65 12.3

L243B 453.6 347.3 74.22 11  
 L484 407.5 301.2 64.37 10  
 TOTAL NUMBER OF LABORATORIES REPORTING


The following laboratories were omitted from the grand means because of extreme test results:

ANALYSIS T40-2 TABLE 2  
AIR RESISTANCE. SHEFFIELD UNITS (CC/MIN) FOR 0.442 SQ. IN (3/4 IN. DIA) GRIFFICE  
SHEFFIELD TESTER IS STANDARD FOR THIS ANALYSIS

LAB CODE	MEANS F	J47 B73	COORDINATES MAJOR	MINOR	Avg R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L626	6	98.4	148.6	-11.9	2.6	.78 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L249	6	99.6	152.8	-7.7	3.5	1.18 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L223	6	99.6	161.6	.1	7.6	1.26 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L230S	6	99.7	147.2	-12.6	.8	1.05 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L158	6	100.0	151.0	-9.1	2.3	.87 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L390	6	101.3	152.9	-6.8	2.1	1.27 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L312	6	101.4	159.8	-.6	5.2	.59 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L262S	6	101.5	140.4	-17.7	-4.0	.75 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L318	6	101.8	155.8	-4.0	3.0	1.09 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L349	6	101.9	152.6	-6.8	1.4	.91 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L370	6	102.7	160.8	.9	4.5	.95 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L124S	6	103.1	151.6	-7.1	-.1	1.42 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L173B	6	104.0	158.0	-1.0	2.1	.78 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L121	6	104.3	160.8	1.6	3.1	1.21 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L132	6	104.4	158.7	-.2	2.0	.94 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L352	6	104.7	151.9	-6.1	-1.4	.90 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L190C	6	105.3	156.0	-2.2	-.0	1.14 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L360	6	105.3	147.7	-9.5	-3.9	.87 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L233	6	105.6	155.0	-2.9	-.7	1.00 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L575	6	106.9	169.4	10.4	4.8	1.09 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L157	6	107.4	152.2	-4.5	-3.6	.90 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L255	6	107.7	161.9	4.2	.6	1.00 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L597	6	108.0	167.5	9.3	3.0	.95 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L257B	6	108.2	163.7	6.0	1.0	1.14 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L127	6	108.5	152.2	-4.0	-4.6	.77 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L260	6	109.1	165.3	7.8	1.0	.96 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L122S	6	109.1	156.2	-.2	-3.3	1.22 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L354	6	109.2	151.6	-4.2	-5.5	.88 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L587	6	109.9	164.3	7.3	-.2	1.18 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L148	6	110.0	159.8	3.4	-2.4	1.06 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L305	6	110.2	159.0	2.8	-2.9	.68 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L114	6	110.5	166.8	9.8	.5	1.15 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L257C	6	110.9	159.3	3.4	-3.4	.75 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L257A	6	110.9	157.5	1.8	-4.3	.88 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L288	6	113.8	169.4	13.6	-1.2	1.26 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L301	6	114.1	172.1	16.2	-.2	1.40 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L241	6	115.0	164.0	9.4	-4.8	1.15 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L213	6	115.7	165.8	11.4	-4.6	.62 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L228	#	131.1	191.4	41.2	-6.2	1.32 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L562	#	293.0	338.0	246.5	-80.7	3.57 40S AIR RESISTANCE, SHEFFIELD (3/4 INCH DIAMETER GRIFFICE)
L484	*	407.5	684.0	605.9	-19.8	2.60 40B AIR RESISTANCE, BENDTSSEN, WG 150
L182B	*	413.5	727.5	647.1	-4.8	4.28 40B AIR RESISTANCE, BENDTSSEN, WG 150
L243B	*	453.6	814.9	743.1	.7	4.87 40B AIR RESISTANCE, BENDTSSEN, WG 150
GMEANS:	106.3	157.9			1.00	
95% ELLIPSE:	20.3	8.5			WITH GAMMA = 62 DEGREES	

# AIR RESISTANCE, SHEFFIELD

SAMPLE J47 = 106. SHEFF. UNITS SAMPLE E73 = 158. SHEFF. UNITS

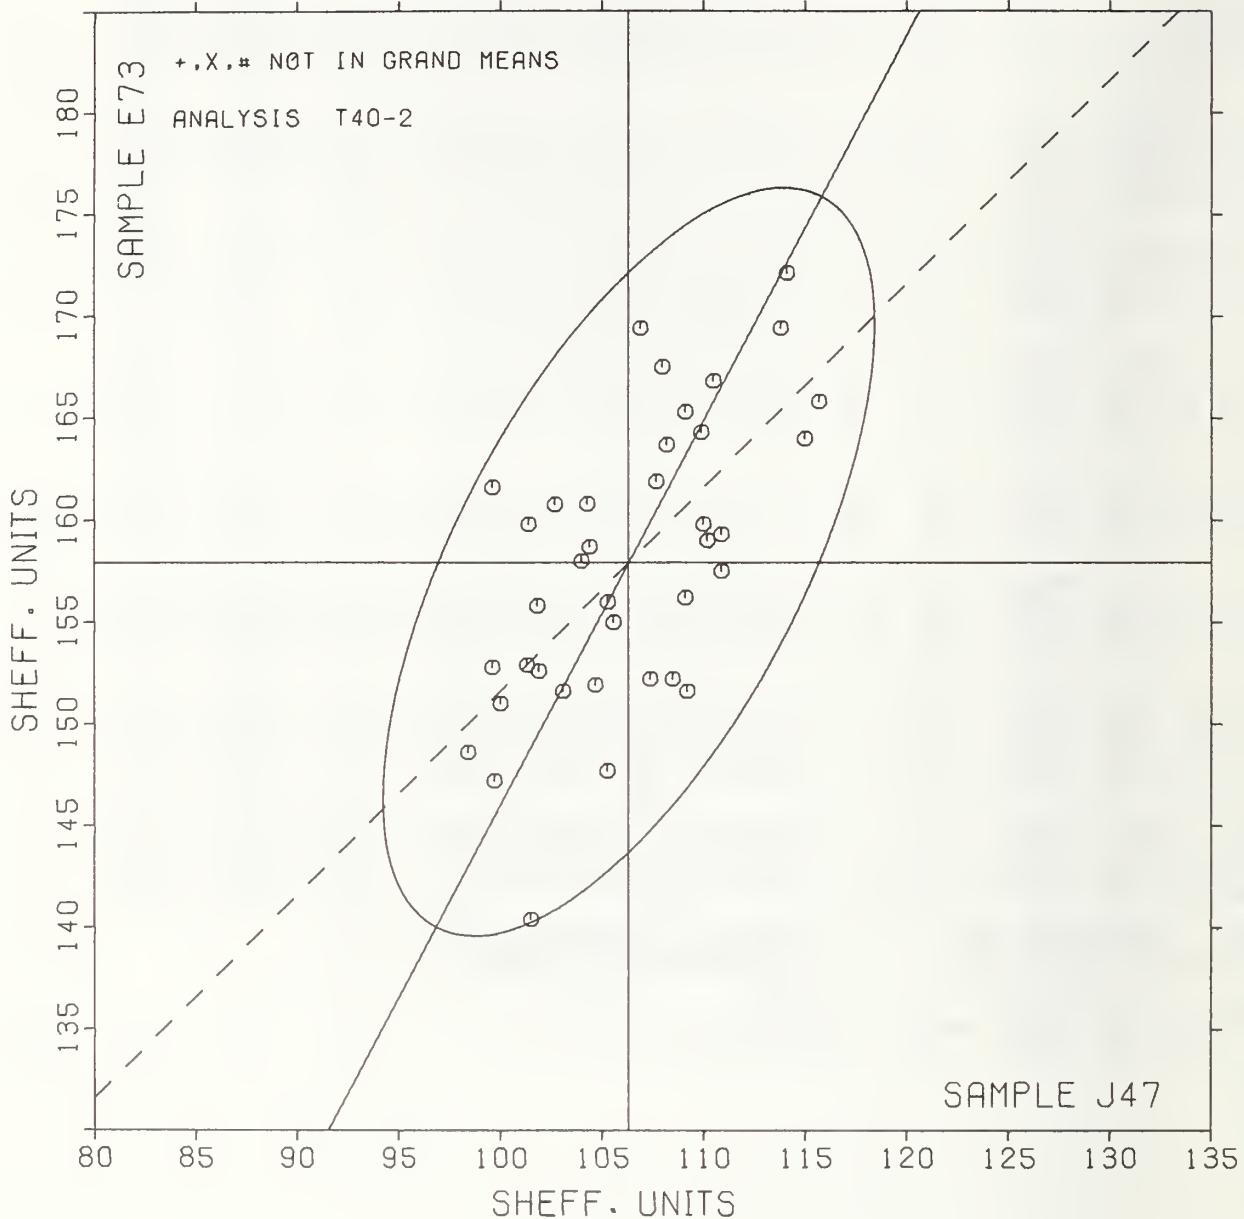

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T41-1 TABLE 1  
AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation  
DIRECT READING, SEC/10 CC, MERCURY DENSITY

JUNE 1978

LAB CODE	SAMPLE E37	BLEACHED BACKING				SAMPLE B73	RELEASE BASE				TEST D. = 10		
		MEAN	DEV	N.DEV	SDR		MEAN	DEV	N.DEV	SDR	R.SDR	VAR	F
L122	813.	.59.	1.51	87.	1.11	1200.	123.	.49	340.	.82	41G	0	L122
L128	712.	-43.	-1.11	54.	.68	934.	-144.	-58	197.	.47	41G	0	L128
L166M	759.	.4.	.11	69.	.88	1423.	345.	1.39	557.	1.34	41G	0	L166M
L195	676.	-79.	-2.03	119.	1.51	872.	-206.	-83	418.	1.01	41G	0	L195
L224	779.	25.	.64	69.	.88	1429.	351.	1.42	791.	1.91	41G	0	L224
L230	746.	-8.	.22	91.	1.16	1348.	271.	1.09	773.	1.86	41G	0	L230
L259	17997.	17242.	444.74	1591.	20.23	26442.	25364.	102.33	9479.	22.85	41G	#	L259
L358	778.	23.	.60	62.	.79	1120.	42.	.17	470.	1.13	41G	0	L358
L396T	723.	-31.	.81	84.	1.07	700.	-378.	-1.52	105.	.25	41G	0	L396T
L557	762.	7.	.19	69.	.88	1119.	41.	.17	463.	1.12	41G	0	L557
L558	747.	-8.	.20	95.	1.21	1248.	170.	.69	565.	1.36	41G	0	L558
L559	813.	58.	1.50	47.	.59	763.	-315.	-1.27	157.	.38	41G	0	L559
L561	731.	-24.	.62	79.	1.00	1036.	-42.	-1.17	352.	.85	41G	0	L561
L576	771.	17.	.43	98.	1.24	818.	-259.	-1.05	206.	.50	41G	0	L576

GR. MEAN = 755. SEC/10 CC  
SD MEANS = 39. SEC/10 CC

GRAND MEAN = 1078. SEC/10 CC  
SD OF MEANS = 248. SEC/10 CC

TEST DETERMINATIONS = 10  
13 LABS IN GRAND MEANS

AVERAGE SDR = 79. SEC/10 CC

AVERAGE SDR = 415. SEC/10 CC

TOTAL NUMBER OF LABORATORIES REPORTING = 14

Best values: E37 760  $\pm$  60 second per 10 c c,  
B73 1100  $\pm$  330 mercury density  
(direct reading)

The values reported here are the time in seconds required for the displacement of 10 ml of air through an area of 1.0 in.  $^2$  of the specimen. The values are not converted to 100 ml of air nor to oil density.

Data from the following laboratories appear to be off by a multiplicative factor: 259

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T41-1 TABLE 2  
AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation  
DIRECT READING, SEC/10 CC, MERCURY DENSITY

JUNE 1978


LAB CODE	MEANS E37	COORDINATES B73	MAJOR	MINOR	AVG R.SDR	PROPERTY---TEST INSTRUMENT---CONDITIONS	TEST D. = 10	
							VAR	TEST D. = 10
L195	6	676.	872.	-209.	71.	1.26 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L128	0	712.	934.	-145.	37.	.58 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L396T	0	723.	700.	-379.	17.	.66 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L561	0	731.	1036.	-43.	22.	.92 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L230	0	746.	1348.	270.	19.	1.51 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L558	0	747.	1248.	170.	14.	1.29 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L166M	0	759.	1423.	345.	9.	1.11 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L557	0	762.	1119.	42.	.6.	1.00 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L576	0	771.	818.	-259.	-27.	.87 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L358	0	778.	1120.	43.	.22.	.96 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L224	0	779.	1429.	352.	-11.	1.39 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L559	0	813.	763.	-313.	-70.	.49 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L122	0	813.	1200.	125.	-54.	.97 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		
L259	#	17997.	26442.	26007.	-16257.	21.54 41G AIR RESISTANCE, HIGH RANGE, GURLEY MERCURY FLotation		

GMEANS: 755. 1078.  
95% ELLIPSE: 731. 111. WITH GAMMA = 67 DEGREES

AIR RESISTANCE, GURLEY HG FLOTATION

SAMPLE E37 = 755. SEC/10 CC

SAMPLE B73 = 1078. SEC/10 CC

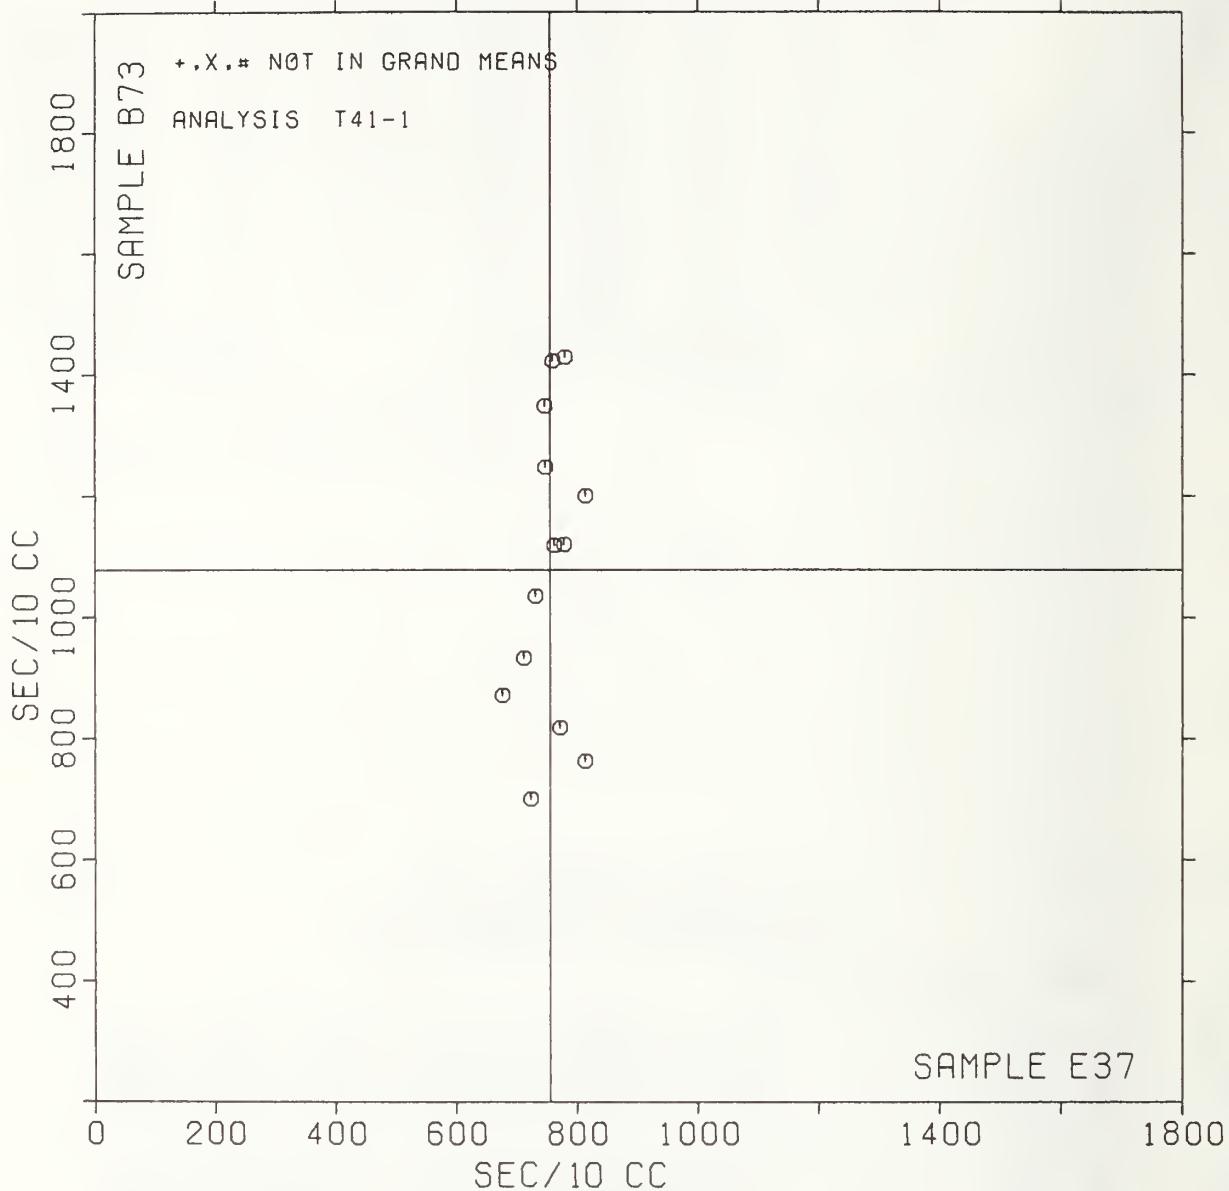

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T44-1 TABLE 1  
 SMOOTHNESS, PARKER PRINTSURF

JUNE 1978

LAB CODE	SAMPLE H45	PRINTING 84 GRAMS PER SQUARE METER					SAMPLE J12	PRINTING 149 GRAMS PER SQUARE METER					TEST D. = 10		
		MEAN	DEV	N. DEV	SDR	R. SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L122	6.80	.85	1.86	.12	1.12		5.54	.49	1.72	.23	1.01		44P	6	L122
L136	5.66	-.29	-.64	.07	.67		4.87	-.18	-.65	.16	.71		44P	6	L136
L182	6.12	.17	.38	.11	1.06		5.19	.14	.47	.28	1.20		44P	6	L182
L223	5.79	-.16	-.36	.08	.72		4.82	-.24	-.83	.23	1.00		44P	6	L223
L288	5.89	-.06	-.14	.14	1.31		5.12	.07	.23	.25	1.10		44P	6	L288
L317	6.06	.11	.23	.13	1.21		5.14	.09	.30	.24	1.05		44P	6	L317
L588	5.34	-.61	-.134	.10	.92		4.70	-.35	-.125	.21	.92		44P	6	L588
GR. MEAN = 5.95 MICRONS		GRAND MEAN = 5.05 MICRONS					TEST DETERMINATIONS = 10 7 LABS IN GRAND MEANS								
SD MEANS = .46 MICRONS		SD OF MEANS = .28 MICRONS					AVERAGE SDR = .10 MICRONS								
TOTAL NUMBER OF LABORATORIES REPORTING = 7							AVERAGE SDR = .23 MICRONS								
Best values: H45 5.9 microns															
J12 5.1 microns															

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T44-1 TABLE 2  
 SMOOTHNESS, PARKER PRINTSURF

JUNE 1978

LAB CODE	F	MEANS		COORDINATES		AVG R. SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS			
		H45	J12	MAJOR	MINOR		PARKER PRINTSURF	PARKER PRINTSURF	PARKER PRINTSURF	PARKER PRINTSURF
L588	6	5.34	4.70	-.71	.02	.92	44P SMOOTHNESS,	PARKER PRINTSURF		
L136	6	5.66	4.87	-.35	-.00	.69	44P SMOOTHNESS,	PARKER PRINTSURF		
L223	6	5.79	4.82	-.26	-.12	.86	44P SMOOTHNESS,	PARKER PRINTSURF		
L288	6	5.89	5.12	-.02	.09	1.20	44P SMOOTHNESS,	PARKER PRINTSURF		
L317	6	6.06	5.14	.14	.02	1.13	44P SMOOTHNESS,	PARKER PRINTSURF		
L182	6	6.12	5.19	.22	.03	1.13	44P SMOOTHNESS,	PARKER PRINTSURF		
L122	6	6.80	5.54	.98	-.03	1.07	44P SMOOTHNESS,	PARKER PRINTSURF		
GMEANS: 5.95 5.05		95% ELLIPSE: 2.00		1.00		WITH GAMMA = 31 DEGREES				

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T45-1 TABLE 1  
SMOOTHNESS, SHEFFIELD UNITS  
SHEFFIELD TESTER IS STANDARD FOR THIS ANALYSIS

JUNE 1978

LAB CODE	SAMPLE H45 MEAN	PRINTING				SAMPLE J12 MEAN	PRINTING				TEST D. = 15		
		84 GRAMS DEV	N.DEV	SDR	R.SDR		149 GRAMS DEV	N.DEV	SDR	R.SDR	VAR	F	LAB
L107	275.3	12.4	1.27	13.7	1.51	159.3	16.4	2.46	12.4	1.11	45S	6	L107
L108	257.9	=5.0	=.51	5.3	.58	154.1	11.2	1.68	10.4	.94	45S	6	L108
L114	270.7	7.8	.79	9.0	1.00	143.0	.0	.01	14.3	1.29	45S	6	L114
L115	252.3	=10.6	=1.08	8.6	.95	150.7	7.7	1.16	12.1	1.09	45S	6	L115
L121	262.0	.9	=.09	11.6	1.28	142.5	=.5	=.08	16.9	1.52	45S	6	L121
L122	277.7	14.8	1.51	7.5	.83	138.1	=4.9	=.74	8.5	.76	45S	6	L122
L123	256.7	=6.2	=.64	9.2	1.02	138.3	=4.7	=.71	14.5	1.30	45S	6	L123
L124	210.1	=52.8	=5.39	8.5	.94	131.1	=11.8	=1.78	8.4	.76	45S	#	L124
L125	263.3	.4	.04	17.3	1.91	139.0	=4.0	=.60	11.1	.99	45S	6	L125
L126	275.0	12.1	1.23	9.6	1.06	142.0	=1.0	=.15	9.8	.88	45S	6	L126
L128	268.0	5.1	.52	8.6	.95	145.3	2.4	.36	8.3	.75	45S	6	L128
L132	272.7	9.8	1.00	11.2	1.23	144.4	1.4	.22	13.9	1.25	45S	6	L132
L139S	258.3	=4.6	=.47	8.2	.90	156.3	13.4	2.01	10.3	.92	45S	6	L139S
L148	266.5	3.6	.36	6.1	.67	152.6	9.6	1.45	11.9	1.07	45S	6	L148
L152	253.1	=9.8	=1.00	7.0	.77	148.0	5.0	.76	11.0	.99	45S	6	L152
L153	284.1	21.2	2.17	5.6	.61	158.1	15.1	2.27	16.3	1.47	45S	*	L153
L157	272.6	9.7	.99	13.6	1.51	144.0	1.0	.16	6.8	.61	45S	6	L157
L158	252.0	=10.9	=1.11	9.8	1.08	134.3	=8.6	=1.30	11.6	1.05	45S	6	L158
L159	266.9	4.0	.40	9.0	.99	146.1	3.1	.47	12.5	1.13	45S	6	L159
L162	262.3	.6	=.06	4.2	.46	138.7	=4.3	=.65	9.5	.86	45S	6	L162
L166	247.9	=15.0	=1.53	6.8	.75	136.7	=6.2	=.94	12.5	1.12	45S	6	L166
L167	249.7	=13.2	=1.35	14.2	1.57	148.3	5.4	.81	5.2	.47	45S	6	L167
L173B	258.3	=4.6	=.47	7.5	.83	146.7	3.7	.56	12.1	1.08	45S	6	L173B
L176S	267.3	.4	.44	7.1	.79	142.9	=.1	=.02	13.3	1.20	45S	6	L176S
L190C	248.9	=14.0	=1.43	8.0	.88	140.1	=2.9	=.44	13.3	1.20	45S	6	L190C
L190R	246.2	=16.7	=1.70	6.6	.73	134.2	=8.8	=1.32	10.5	.94	45S	6	L190R
L195	246.7	=16.2	=1.65	7.1	.78	139.7	=3.2	=.49	15.3	1.37	45S	6	L195
L203	256.7	=6.2	=.64	10.3	1.14	138.7	=4.2	=.64	13.1	1.18	45S	6	L203
L211	249.0	=13.9	=1.42	18.0	1.99	143.2	.2	.04	11.4	1.02	45S	6	L211
L213	227.0	=35.9	=3.66	7.9	.87	131.0	=12.0	=1.80	10.4	.93	45S	X	L213
L223	258.8	=4.1	=.42	9.3	1.03	134.6	=8.4	=1.26	9.2	.83	45S	6	L223
L224	320.3	57.4	5.86	9.0	.99	155.3	12.4	1.86	10.3	.93	45S	#	L224
L228	280.7	17.8	1.82	9.0	1.00	151.5	8.5	1.28	8.9	.80	45S	6	L228
L230S	265.7	2.8	.28	9.6	1.06	145.1	2.2	.33	13.4	1.21	45S	6	L230S
L231	271.7	8.8	.90	12.0	1.32	153.5	10.6	1.59	10.3	.93	45S	6	L231
L233	261.9	=1.0	=.10	9.8	1.08	144.9	1.9	.29	8.5	.76	45S	6	L233
L241	331.7	68.8	7.02	7.9	.88	165.0	22.0	3.31	9.1	.82	45S	#	L241
L249	260.3	=2.6	=.27	7.3	.80	143.4	.4	.07	14.2	1.28	45S	6	L249
L254	265.9	3.0	.31	8.1	.90	150.2	7.2	1.09	12.2	1.10	45S	6	L254
L255	258.6	=4.3	=.44	3.4	.37	147.5	4.5	.68	11.3	1.02	45S	6	L255
L257A	261.3	=1.6	=.16	10.9	1.20	135.2	=7.8	=1.17	5.7	.51	45S	6	L257A
L257B	268.9	6.0	.61	12.6	1.39	142.5	.5	=.08	11.1	1.00	45S	6	L257B
L257C	257.3	=5.6	=.57	9.0	1.00	140.9	=2.1	=.32	7.0	.63	45S	6	L257C
L259	280.1	17.2	1.76	10.2	1.13	152.8	9.8	1.48	12.1	1.09	45S	6	L259
L260	256.8	=6.1	=.62	7.5	.83	145.3	2.4	.36	11.9	1.07	45S	6	L260
L261	258.8	=4.1	=.42	8.3	.91	135.4	=7.6	=1.14	6.4	.58	45S	6	L261
L262	261.1	=1.8	=.19	6.2	.68	138.8	=4.2	=.63	6.1	.55	45S	6	L262
L275	269.0	6.1	.62	7.4	.81	147.0	4.0	.61	12.2	1.10	45S	6	L275
L278	265.3	2.4	.25	9.2	1.02	151.1	8.1	1.22	6.9	.62	45S	6	L278
L281	263.2	.3	.03	12.7	1.40	144.0	1.0	.16	17.0	1.53	45S	6	L281
L285	263.3	.4	.04	13.2	1.46	135.3	=7.6	=1.15	16.2	1.46	45S	6	L285
L288	267.5	4.6	.47	4.7	.52	142.5	.5	=.08	12.2	1.10	45S	6	L288
L290	239.0	=23.9	=2.44	10.0	1.11	132.7	=10.3	=1.55	9.2	.83	45S	*	L290
L291S	272.5	9.6	.98	6.5	.72	148.5	5.5	.83	12.1	1.09	45S	6	L291S
L297	260.3	=2.6	=.26	6.1	.68	147.7	4.7	.71	12.4	1.11	45S	6	L297
L301	NO DATA REPORTED FOR SAMPLE H45					145.7	2.8	.42	12.3	1.11	45S	M	L301
L305	262.7	.2	.02	9.6	1.06	136.3	=6.6	=1.00	8.1	.73	45S	6	L305
L308	257.6	=5.3	=.54	9.4	1.04	141.3	=1.6	=.25	15.9	1.43	45S	6	L308
L312	274.7	11.8	1.20	6.4	.71	142.7	.3	=.05	14.1	1.27	45S	6	L312
L317	266.1	3.2	.32	10.2	1.12	135.2	=7.8	=1.17	11.6	1.05	45S	6	L317
L318	263.7	.8	.08	10.7	1.18	137.3	=5.6	=.85	14.6	1.32	45S	6	L318
L321	254.0	=8.9	=.91	10.6	1.17	127.7	=15.3	=2.30	7.3	.66	45S	6	L321
L323	275.7	12.8	1.30	9.8	1.08	139.7	=3.3	=.50	11.4	1.03	45S	6	L323
L326	295.9	33.0	3.36	5.7	.63	140.8	=2.2	=.33	9.4	.84	45S	X	L326
L328	269.0	6.1	.62	9.1	1.01	144.3	1.4	.21	12.0	1.08	45S	6	L328

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T45-1 TABLE 1  
SMOOTHNESS, SHEFFIELD UNITS  
SHEFFIELD TESTER IS STANDARD FOR THIS ANALYSIS

JUNE 1978

LAB CODE	SAMPLE H45 MBAN	PRINTING 84 GRAMS PER SQUARE METER					SAMPLE J12 149 GRAMS PER SQUARE METER					TEST D.O. 15		
		DEV	N. DEV	SDR	R. SDR	MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB	
L341	257.7	+5.2	.53	6.6	.72	138.1	+4.8	.73	11.3	1.02	45S	Ø	L341	
L342	275.7	12.8	1.30	12.4	1.37	143.6	.6	.10	9.3	.84	45S	Ø	L342	
L349	266.2	3.3	.34	11.1	1.22	135.7	+7.2	+1.09	11.3	1.01	45S	Ø	L349	
L352	282.3	19.4	1.98	8.1	.89	150.5	7.5	1.13	14.9	1.34	45S	Ø	L352	
L350	259.4	+3.5	.36	7.1	.78	136.1	+6.8	+1.03	7.2	.65	45S	Ø	L360	
L366	260.9	+2.0	.21	10.1	1.12	144.1	1.2	.18	14.9	1.34	45S	Ø	L366	
L370	250.3	-12.6	+1.29	6.9	.76	136.3	+6.7	+1.01	10.6	.95	45S	Ø	L370	
L372	260.5	+2.4	.24	4.8	.53	156.3	13.4	2.01	8.3	.75	45S	Ø	L372	
L376	253.3	+9.6	+0.98	10.6	1.17	148.0	5.0	.76	15.1	1.36	45S	Ø	L376	
L380	260.0	+2.9	.30	4.2	.47	131.0	+12.0	+1.80	7.8	.71	45S	Ø	L380	
L382	251.5	+11.4	+1.16	4.2	.46	136.1	+6.8	+1.03	10.6	.95	45S	Ø	L382	
L390	254.3	+8.6	.88	9.4	1.04	134.2	+8.8	+1.32	11.4	1.03	45S	Ø	L390	
L396M	266.3	3.4	.35	9.3	1.03	140.3	+2.6	+0.40	12.7	1.15	45S	Ø	L396M	
L554	263.9	1.0	.10	9.6	1.06	144.1	1.2	.18	6.8	.62	45S	Ø	L554	
L561	304.0	41.1	4.19	6.3	.70	150.0	7.0	1.06	6.5	.59	45S	#	L561	
L575	280.2	17.3	1.76	10.7	1.18	141.7	+1.2	.19	10.6	.95	45S	Ø	L575	
L587	258.3	+4.6	.47	11.4	1.26	142.0	+1.0	.15	8.6	.78	45S	Ø	L587	
L597	288.1	25.2	2.57	4.2	.46	146.9	3.9	.59	9.7	.87	45S	#	L597	
L607	249.3	+13.6	+1.38	8.0	.88	149.5	6.5	.98	7.3	.65	45S	Ø	L607	
L626	258.7	+4.2	.43	10.8	1.20	136.7	+6.2	+0.94	9.5	.86	45S	Ø	L626	
GR. MEAN	262.9	SHEFF. UNITS				GRAND MEAN	143.0	SHEFF. UNITS			TEST DETERMINATIONS	*	15	
SD MEANS	9.8	SHEFF. UNITS				SD OF MEANS	6.7	SHEFF. UNITS			78 LABS IN GRAND MEANS			
AVERAGE SDR	9.1	SHEFF. UNITS				AVERAGE SDR	11.1	SHEFF. UNITS						
L174	307.1	44.2	4.51	5.9	.65	231.1	88.1	13.24	7.8	.70	45R	*	L174	
TOTAL NUMBER OF LABORATORIES REPORTING	86													

Best values: H45 265 + 16 Sheffield units  
J12 140 + 11 Sheffield units

The following laboratories were omitted from the grand means because of extreme test results: 124, 224, 241, 561

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T45-1 TABLE 2  
SMOOTHNESS, SHEFFIELD UNITS  
SHEFFIELD TESTER IS STANDARD FOR THIS ANALYSIS

LAB CODE	F	MEANS H45	J12	COORDINATES MAJOR	MINOR	Avg R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L301	M	145.7				1.11 45S	SMOOTHNESS, SHEFFIELD
L124	#	210.1	131.1	-53.4	9.0	.85 45S	SMOOTHNESS, SHEFFIELD
L213	X	227.0	131.0	-37.8	2.5	.90 45S	SMOOTHNESS, SHEFFIELD
L290	*	239.0	132.7	-26.0	.5	.97 45S	SMOOTHNESS, SHEFFIELD
L190R	G	246.2	134.2	-18.8	-1.8	.84 45S	SMOOTHNESS, SHEFFIELD
L195	G	246.7	139.7	-16.2	3.1	1.08 45S	SMOOTHNESS, SHEFFIELD
L166	G	247.9	136.7	-16.2	.1	.94 45S	SMOOTHNESS, SHEFFIELD
L190C	G	248.9	140.1	-14.0	2.6	1.04 45S	SMOOTHNESS, SHEFFIELD
L211	G	249.0	143.2	-12.8	5.5	1.51 45S	SMOOTHNESS, SHEFFIELD
L607	G	249.3	149.5	-10.1	11.1	.77 45S	SMOOTHNESS, SHEFFIELD
L167	G	249.7	148.3	-10.2	10.0	1.02 45S	SMOOTHNESS, SHEFFIELD
L370	G	250.3	136.3	-14.2	-1.4	.86 45S	SMOOTHNESS, SHEFFIELD
L382	G	251.5	136.1	-13.1	-2.0	.71 45S	SMOOTHNESS, SHEFFIELD
L158	G	252.0	134.3	-13.4	-3.9	1.06 45S	SMOOTHNESS, SHEFFIELD
L115	G	252.3	150.7	-6.9	11.1	1.02 45S	SMOOTHNESS, SHEFFIELD
L152	G	253.1	148.0	-7.2	8.4	.88 45S	SMOOTHNESS, SHEFFIELD
L376	G	253.3	148.0	-7.0	8.3	1.27 45S	SMOOTHNESS, SHEFFIELD
L321	G	254.0	127.7	-14.0	-10.8	.91 45S	SMOOTHNESS, SHEFFIELD
L390	G	254.3	134.2	-11.3	-4.8	1.03 45S	SMOOTHNESS, SHEFFIELD
L203	G	256.7	138.7	-7.4	-1.6	1.16 45S	SMOOTHNESS, SHEFFIELD
L123	G	256.7	138.3	-7.6	-2.0	1.16 45S	SMOOTHNESS, SHEFFIELD
L260	G	256.8	145.3	-4.8	4.5	.95 45S	SMOOTHNESS, SHEFFIELD
L257C	G	257.3	140.9	-6.0	.2	.81 45S	SMOOTHNESS, SHEFFIELD
L308	G	257.6	141.3	-5.5	.5	1.23 45S	SMOOTHNESS, SHEFFIELD
L341	G	257.7	138.1	-6.6	-2.5	.87 45S	SMOOTHNESS, SHEFFIELD
L108	G	257.9	154.1	.4	12.2	.76 45S	SMOOTHNESS, SHEFFIELD
L587	G	258.3	142.0	-4.6	.8	1.02 45S	SMOOTHNESS, SHEFFIELD
L139S	G	258.3	156.3	.8	14.1	.91 45S	SMOOTHNESS, SHEFFIELD
L173B	G	258.3	146.7	-2.8	5.2	.96 45S	SMOOTHNESS, SHEFFIELD
L255	G	258.6	147.5	-2.3	5.8	.70 45S	SMOOTHNESS, SHEFFIELD
L626	G	258.7	136.7	-6.3	-4.2	1.03 45S	SMOOTHNESS, SHEFFIELD
L223	G	258.8	134.6	-7.0	-6.2	.93 45S	SMOOTHNESS, SHEFFIELD
L261	G	258.8	135.4	-6.7	-5.5	.75 45S	SMOOTHNESS, SHEFFIELD
L360	G	259.4	136.1	-5.8	-5.0	.72 45S	SMOOTHNESS, SHEFFIELD
L380	G	260.0	131.0	-7.2	-10.0	.59 45S	SMOOTHNESS, SHEFFIELD
L249	G	260.3	143.4	-2.3	1.4	1.04 45S	SMOOTHNESS, SHEFFIELD
L297	G	260.3	147.7	-.6	5.3	.89 45S	SMOOTHNESS, SHEFFIELD
L372	G	260.5	156.3	2.9	13.3	.64 45S	SMOOTHNESS, SHEFFIELD
L366	G	260.9	144.1	-1.4	1.9	1.23 45S	SMOOTHNESS, SHEFFIELD
L262	G	261.1	136.8	-3.3	-3.2	.61 45S	SMOOTHNESS, SHEFFIELD
L257A	G	261.3	135.2	-4.4	-6.6	.86 45S	SMOOTHNESS, SHEFFIELD
L233	G	261.9	144.9	-.2	2.1	.92 45S	SMOOTHNESS, SHEFFIELD
L121	G	262.0	142.5	-1.0	-.1	1.40 45S	SMOOTHNESS, SHEFFIELD
L162	G	262.3	138.7	-2.2	-3.8	.66 45S	SMOOTHNESS, SHEFFIELD
L305	G	262.7	136.3	-2.7	-6.1	.90 45S	SMOOTHNESS, SHEFFIELD
L281	G	263.2	144.6	.7	.8	1.47 45S	SMOOTHNESS, SHEFFIELD
L125	G	263.3	139.0	-1.1	-3.8	1.45 45S	SMOOTHNESS, SHEFFIELD
L285	G	263.3	135.3	-2.5	-7.2	1.46 45S	SMOOTHNESS, SHEFFIELD
L318	G	263.7	137.3	-1.4	-5.5	1.25 45S	SMOOTHNESS, SHEFFIELD
L554	G	263.9	144.1	1.4	.7	.84 45S	SMOOTHNESS, SHEFFIELD
L278	G	265.3	151.1	5.3	6.6	.82 45S	SMOOTHNESS, SHEFFIELD
L230S	G	265.7	145.1	3.4	1.0	1.14 45S	SMOOTHNESS, SHEFFIELD
L254	G	265.9	150.2	5.5	5.6	1.00 45S	SMOOTHNESS, SHEFFIELD
L317	G	266.1	135.2	-.0	-8.4	1.08 45S	SMOOTHNESS, SHEFFIELD
L349	G	266.2	135.7	.3	-7.9	1.12 45S	SMOOTHNESS, SHEFFIELD
L396M	G	266.3	140.3	2.2	-3.7	1.09 45S	SMOOTHNESS, SHEFFIELD
L148	G	266.5	152.6	6.9	7.6	.87 45S	SMOOTHNESS, SHEFFIELD
L159	G	266.9	146.1	4.8	1.4	1.06 45S	SMOOTHNESS, SHEFFIELD
L176S	G	267.3	142.9	4.0	-1.7	.99 45S	SMOOTHNESS, SHEFFIELD
L288	G	267.5	142.5	4.0	-2.2	.81 45S	SMOOTHNESS, SHEFFIELD
L128	G	268.0	145.3	5.6	.3	.85 45S	SMOOTHNESS, SHEFFIELD
L257B	G	268.9	142.5	5.4	-2.7	1.20 45S	SMOOTHNESS, SHEFFIELD
L275	G	269.0	147.0	7.2	1.4	.96 45S	SMOOTHNESS, SHEFFIELD
L328	G	269.0	144.3	6.2	-1.0	1.04 45S	SMOOTHNESS, SHEFFIELD
L114	G	270.7	143.0	7.2	-2.9	1.14 45S	SMOOTHNESS, SHEFFIELD


TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T45-1 TABLE 2  
 SMOOTHNESS, SHEFFIELD UNITS  
 SHEFFIELD TESTER IS STANDARD FOR THIS ANALYSIS

JUNE 1978

LAB CODE	F	MEANS R45	J12	COORDINATES MAJOR	MINOR	R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L231	6	271.7	153.5	12.2	6.4	1.13	45S SMOOTHNESS, SHEFFIELD
L291S	6	272.5	148.5	10.9	1.5	.90	45S SMOOTHNESS, SHEFFIELD
L157	6	272.6	144.0	9.4	-2.7	1.06	45S SMOOTHNESS, SHEFFIELD
L132	6	272.7	144.4	9.6	-2.4	1.24	45S SMOOTHNESS, SHEFFIELD
L312	6	274.7	142.7	10.8	-4.7	.99	45S SMOOTHNESS, SHEFFIELD
L126	6	275.0	142.0	10.8	-5.5	.97	45S SMOOTHNESS, SHEFFIELD
L107	6	275.3	159.3	17.7	10.5	1.31	45S SMOOTHNESS, SHEFFIELD
L342	6	275.7	143.6	12.1	-4.2	1.11	45S SMOOTHNESS, SHEFFIELD
L323	6	275.7	139.7	10.6	-7.9	1.05	45S SMOOTHNESS, SHEFFIELD
L122	6	277.7	138.1	11.8	-10.1	.80	45S SMOOTHNESS, SHEFFIELD
L259	6	280.1	152.8	19.7	2.6	1.11	45S SMOOTHNESS, SHEFFIELD
L575	6	280.2	141.7	15.5	-7.7	1.06	45S SMOOTHNESS, SHEFFIELD
L228	6	280.7	151.5	19.7	1.1	.90	45S SMOOTHNESS, SHEFFIELD
L352	6	282.3	150.5	20.8	-4	1.12	45S SMOOTHNESS, SHEFFIELD
L153	*	284.1	158.1	25.4	6.0	1.04	45S SMOOTHNESS, SHEFFIELD
L597	*	288.1	146.9	24.8	-5.9	.67	45S SMOOTHNESS, SHEFFIELD
L326	X	295.9	140.8	29.7	-14.5	.73	45S SMOOTHNESS, SHEFFIELD
L561	#	304.0	150.0	40.7	-9.0	.64	45S SMOOTHNESS, SHEFFIELD
L174	*	307.1	231.1	74.3	64.8	.67	45R SMOOTHNESS, SHEFFIELD, NON-STANDARD INSTRUMENT
L224	#	320.3	155.3	57.8	-10.3	.96	45S SMOOTHNESS, SHEFFIELD
L241	#	331.7	165.0	72.0	-5.6	.85	45S SMOOTHNESS, SHEFFIELD
GMEANS:		262.9	143.0		1.00		
95% ELLIPSE:		25.9	14.6		WITH GAMMA = 22 DEGREES		

# SMOOTHNESS, SHEFFIELD

SAMPLE H45 = 263. SHEFF. UNITS SAMPLE J12 = 143. SHEFF. UNITS

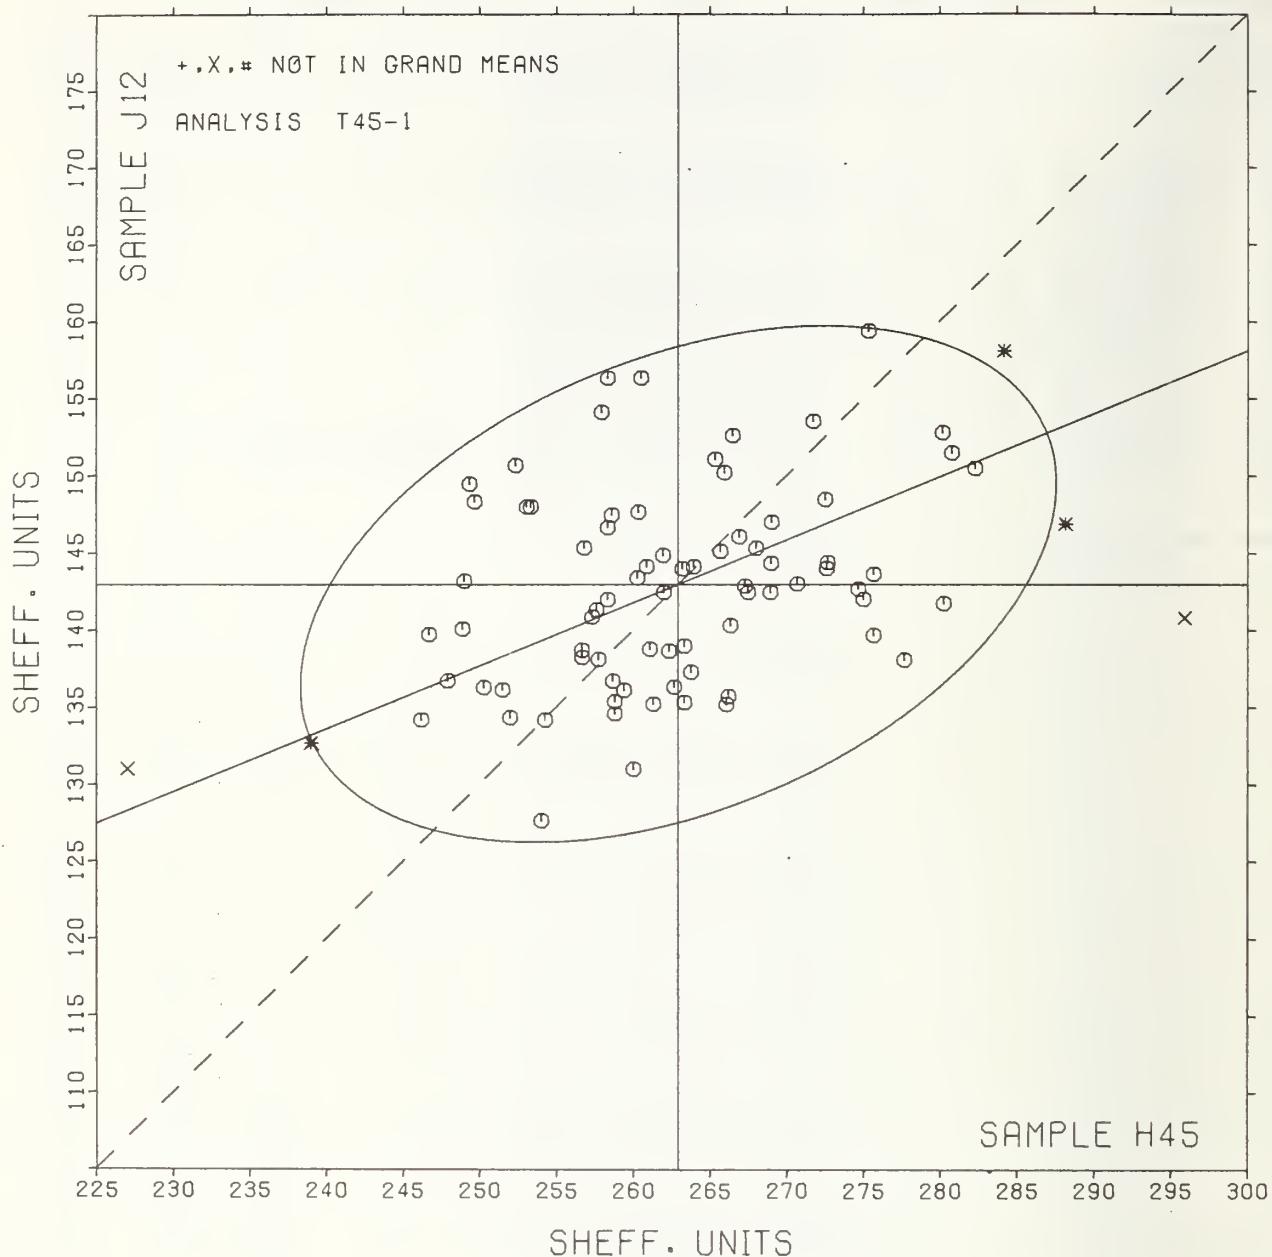

## ANALYSIS T45-2 TABLE 1

## SMOOTHNESS, BEKK SECONDS

TAPPI SUGGESTED METHOD T479 SU-71, SMOOTHNESS OF PAPER (BEKK METHOD)

LAB CODE	SAMPLE H45	PRINTING 84 GRAMS PER SQUARE METER				SAMPLE J12	PRINTING 149 GRAMS PER SQUARE METER				TEST D. = 15		
		MEAN	DEV	N.DEV	SDR		MEAN	DEV	N.DEV	SDR	R.SDR	VAR	F
L139B	16.27	1.06	.84	.59	.74	32.53	.24	.11	4.27	.98	45K	6	L139B
L162	6.44	-8.76	-6.93	.47	.59	26.73	-6.04	-2.68	3.35	.77	45K	#	L162
L176	12.63	-2.58	-2.04	.48	.60	23.55	-9.22	-4.09	2.34	.54	45K	#	L176
L182K	13.25	-1.95	-1.54	.61	.76	29.69	-3.08	-1.37	3.56	.82	45K	6	L182K
L190C	15.43	.23	.18	.81	1.01	34.60	1.82	.81	5.36	1.23	45K	6	L190C
L230B	14.47	-.74	-.58	.92	1.14	35.47	2.69	1.19	3.81	.88	45K	6	L230B
L243K	14.96	-.24	-.19	.55	.69	31.67	-1.11	-.49	4.48	1.03	45K	6	L243K
L291K	17.17	1.97	1.56	1.31	1.63	34.87	2.09	.93	5.14	1.18	45K	6	L291K
L581	14.87	-.34	-.27	.83	1.04	30.60	-2.18	-.97	3.81	.88	45K	6	L581
GR. MEAN = 15.20 BEKK SECONDS						GRAND MEAN = 32.78 BEKK SECONDS					TEST DETERMINATIONS = 15		
SD MEANS = 1.26 BEKK SECONDS						SD OF MEANS = 2.25 BEKK SECONDS					7 LABS IN GRAND MEANS		
AVERAGE SDR = .80 BEKK SECONDS						AVERAGE SDR = 4.35 BEKK SECONDS							
L182G	35.50	20.30	16.06	2.51	3.12	104.17	71.39	31.68	11.50	2.64	45K	6	L182G
L250M	16.57	1.37	1.08	.83	1.04	30.93	-1.84	-.82	2.58	.59	45L	6	L250M
L251	14.13	-1.07	-.85	.77	.95	26.97	-5.81	-2.58	2.83	.65	45L	6	L251
L388	40.67	25.46	20.15	4.89	6.08	202.94	170.16	75.52	26.14	6.01	45H	6	L388
TOTAL NUMBER OF LABORATORIES REPORTING = 13													

Best values: H45 15 Bekk seconds  
J12 31 Bekk seconds

The following laboratories were omitted from the grand means because of extreme test results: 176

Data from the following laboratories appear to be off by a multiplicative factor: 162

## ANALYSIS T45-2 TABLE 2

## SMOOTHNESS, BEKK SECONDS

TAPPI SUGGESTED METHOD T479 SU-71, SMOOTHNESS OF PAPER (BEKK METHOD)

LAB CODE	P	MEANS		COORDINATES		AVG R.SDR	VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
		H45	J12	MAJOR	MINOR			
L162	#	6.44	26.73	-8.77	6.04	.68	45K	SMOOTHNESS, BEKK
L176	#	12.63	23.55	-9.53	-.88	.57	45K	SMOOTHNESS, BEKK
L182K	6	13.25	29.69	-3.57	.72	.79	45K	SMOOTHNESS, BEKK
L251	*	14.13	26.97	-5.81	-1.07	.80	45L	SMOOTHNESS, BEKK, 20 C, 65% RH
L230B	6	14.47	35.47	2.25	1.65	1.01	45K	SMOOTHNESS, BEKK
L581	6	14.87	30.60	-2.15	-.46	.96	45K	SMOOTHNESS, BEKK
L243K	6	14.96	31.67	-1.12	-.17	.86	45K	SMOOTHNESS, BEKK
L190C	6	15.43	34.60	1.79	.43	1.12	45K	SMOOTHNESS, BEKK
L139B	6	16.27	32.53	.15	-1.08	.86	45K	SMOOTHNESS, BEKK
L250M	*	16.57	30.93	-1.23	-1.94	.82	45L	SMOOTHNESS, BEKK, 20 C, 65% RH
L291K	6	17.17	34.87	2.66	-1.10	1.41	45K	SMOOTHNESS, BEKK
L182G	*	35.50	104.17	73.94	6.46	2.88	45H	GURLEY OIL FLOATATION
L388	*	40.67	202.94	168.08	36.81	6.05	45H	GURLEY OIL FLOATATION
GMEANS:		15.20	32.78		1.00			
		95% ELLIPSE:	8.87	3.74		WITH GAMMA = 69 DEGREES		

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T47-1 TABLE 1  
SMOOTHNESS, BENDTSEN

JUNE 1978

LAB CODE	SAMPLE H45	PRINTING 84 GRAMS PER SQUARE METER				SAMPLE J12	PRINTING 149 GRAMS PER SQUARE METER				TEST D. = 10		
		MEAN	DEV	N. DEV	SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F
L176	458.	.2.	.02	9.	.22	175.	.0.	.02	9.	.39	47B	Ø	L176
L182B	577.	117.	.98	69.	1.66	189.	14.	.93	26.	1.08	47B	Ø	L182B
L236	449.	-11.	-.09	26.	.63	184.	9.	.59	23.	.95	47B	Ø	L236
L243B	464.	4.	.03	60.	1.45	166.	-.9.	-.64	20.	.85	47B	Ø	L243B
L244	220.	-240.	-.200	16.	.37	156.	-.20.	-.1.36	23.	.96	47B	Ø	L244
L248	417.	-43.	-.36	37.	.88	165.	-.11.	-.75	24.	1.01	47B	Ø	L248
L280	621.	161.	1.34	83.	1.98	201.	25.	1.69	40.	1.67	47B	Ø	L280
L333	379.	-81.	-.67	38.	.91	162.	-.14.	-.93	32.	1.35	47B	Ø	L333
L484	555.	95.	.79	37.	.88	183.	7.	.49	18.	.74	47B	Ø	L484
GR. MEAN =	460. ML/MIN					GRAND MEAN =	176. ML/MIN					TEST DETERMINATIONS =	10
SD MEANS =	120. ML/MIN					SD OF MEANS =	15. ML/MIN					9 LABS IN GRAND MEANS	
AVERAGE SDR =	42. ML/MIN					AVERAGE SDR =	24. ML/MIN						
TOTAL NUMBER OF LABORATORIES REPORTING =	9												
Best values: H45 460 milliliter per minute						J12 175 milliliter per minute							

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T47-1 TABLE 2  
SMOOTHNESS, BENDTSEN

JUNE 1978

LAB CODE	F	MEANS		COORDINATES		AVG R. SDR	VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
		H45	J12	MAJOR	MINOR			
L244	Ø	220.	156.	-241.	6.	.67	47B	SMOOTHNESS, BENDTSEN, WG 150
L333	Ø	379.	162.	-82.	-5.	1.13	47B	SMOOTHNESS, BENDTSEN, WG 150
L248	Ø	417.	165.	-44.	-6.	.95	47B	SMOOTHNESS, BENDTSEN, WG 150
L236	Ø	449.	184.	-10.	10.	.79	47B	SMOOTHNESS, BENDTSEN, WG 150
L176	Ø	458.	175.	-2.	-0.	.30	47B	SMOOTHNESS, BENDTSEN, WG 150
L243B	Ø	464.	166.	3.	-10.	1.15	47B	SMOOTHNESS, BENDTSEN, WG 150
L484	Ø	555.	183.	95.	-3.	.81	47B	SMOOTHNESS, BENDTSEN, WG 150
L182B	Ø	577.	189.	118.	1.	1.37	47B	SMOOTHNESS, BENDTSEN, WG 150
L280	Ø	621.	201.	163.	7.	1.82	47B	SMOOTHNESS, BENDTSEN, WG 150
GMEANS:		460.	176.		1.00			
95% ELLIPSE:		397.	22.		WITH GAMMA = 6 DEGREES			

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS TS6-1 TABLE 1  
K & N INK ABSORPTION

JUNE 1978

LAB CODE	SAMPLE B80 MEAN	COATED OFFSET 866K				SAMPLE E50 MEAN	OFFSET PRINTING 96 GRAMS PER SQUARE METER				TEST D = 4		
		DEV	N. DEV	SDR	R. SDR		DEV	N. DEV	SDR	R. SDR	VAR	F	LA8
L126	22.32	.087	.029	.82	1.23	59.55	.454	.099	.62	1.88	56K	G	L126
L182	23.05	.115	.05	.79	1.20	64.20	.11	.02	.16	.49	56K	G	L182
L213	14.62	.057	.028	.13	.19	45.72	.1837	.399	2.65	7.99	56K	#	L213
L278	28.37	.518	1.70	.49	.74	68.50	.441	.96	.08	.25	56K	G	L278
L291	20.00	.320	-1.05	.91	1.38	65.15	1.06	.23	.06	.17	56K	G	L291
L339	24.75	1.55	.51	.50	.75	69.25	5.16	1.12	.29	.87	56K	G	L339
L388	20.67	-2.52	.083	.46	.70	57.90	-6.19	-1.34	.77	2.33	56K	G	L388
L616	54.50	31.30	10.26	1.00	1.51	100.00	35.91	7.79	.00	.00	56K	#	L616

GR. MEAN = 23.20 K &amp; N UNITS

GRAND MEAN = 64.09 K &amp; N UNITS

TEST DETERMINATIONS = 4

SD MEANS = 3.05 K &amp; N UNITS

SD OF MEANS = 4.61 K &amp; N UNITS

6 LABS IN GRAND MEANS

AVERAGE SDR = .66 K &amp; N UNITS

AVERAGE SDR =

.33 K &amp; N UNITS

TOTAL NUMBER OF LABORATORIES REPORTING = 8

Best values: B80 23 K & N units  
E50 65 K & N unitsThe following laboratories were omitted from the  
grand means because of extreme test results: 213, 616

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS TS6-1 TABLE 2  
K & N INK ABSORPTION

JUNE 1978

LAB CODE	F	MEANS		COORDINATES		AVG R. SDR	VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS		
		B80	E50	MAJOR	MINOR					
L213	#	14.62	45.72	-20.22	-1.35	4.09	56K INK ABSORPTION, K&N INK TEST			
L291	G	20.00	65.15	-.61	3.31	.77	55K INK ABSORPTION, K&N INK TEST			
L388	G	20.67	57.90	-6.64	-.78	1.52	56K INK ABSORPTION, K&N INK TEST			
L126	G	22.32	59.55	-4.40	-1.43	1.56	56K INK ABSORPTION, K&N INK TEST			
L182	G	23.05	64.20	.02	.18	.84	56K INK ABSORPTION, K&N INK TEST			
L339	G	24.75	69.25	5.27	1.13	.81	56K INK ABSORPTION, K&N INK TEST			
L278	G	28.37	68.50	6.36	-2.41	.49	56K INK ABSORPTION, K&N INK TEST			
L616	#	54.50	100.00	46.55	-10.11	.75	55K INK ABSORPTION, K&N INK TEST			

GMEANS: 23.20 64.09  
95% ELLIPSE: 21.41 8.48 WITH GAMMA = 61 DEGREES

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T57-1 TABLE 1  
 HYDROGEN ION CONCENTRATION (PH), COLD  
 TAPPI STANDARD T509 GS-77

JUNE 1978

LAB CODE	SAMPLE J77	PRINTING 89 GRAMS PER SQUARE METER					SAMPLE J14	PRINTING 89 GRAMS PER SQUARE METER					TEST D.- S		
		MEAN	DEV	N. DEV	SDR	R. SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L174C	7.74	.43	1.23	.09	.96		7.78	.47	1.17	.04	.81		57F	6	L174C
L182C	7.20	-.11	-.30	.11	1.14		6.95	-.36	-.91	.04	.64		57D	6	L182C
L251C	7.38	.08	.22	.03	.34		7.40	.09	.23	.03	.48		57P	6	L251C
L328	7.66	.35	1.00	.15	1.63		7.78	.47	1.17	.04	.81		57M	6	L328
L356	6.87	-.43	-.123	.07	.75		6.93	-.39	-.97	.09	1.62		57V	6	L356
L484A	6.98	-.33	-.92	.11	1.18		7.04	-.27	-.68	.09	1.63		57Y	6	L484A
GR. MEAN =	7.31 PH UNITS						GRAND MEAN =	7.31 PH UNITS					TEST DETERMINATIONS =	5	
SD MEANS =	.35 PH UNITS						SD OF MEANS =	.40 PH UNITS					6 LABS IN GRAND MEANS		
AVERAGE SDR =	.09 PH UNITS						AVERAGE SDR =	.05 PH UNITS							
TOTAL NUMBER OF LABORATORIES REPORTING =	6														

Best values: J77 7.3 pH units  
 J14 7.3 pH units

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T57-1 TABLE 2  
 HYDROGEN ION CONCENTRATION (PH), COLD  
 TAPPI STANDARD T509 GS-77

JUNE 1978

LAB CODE	F	MEANS		COORDINATES		AVG R.SDR	VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS		
		J77	J14	MAJOR	MINOR					
L356	6	6.87	6.93	-.58	.07	1.19	57V PH, COLD, BECKMAN EXPANDOMATIC			
L484A	6	6.98	7.04	-.42	.06	1.40	57Y PH, COLD, BECKMAN MODEL B2			
L182C	6	7.20	6.95	-.34	-.16	.89	57D PH, COLD, RADIOMETER TYPE PH M 28			
L251C	6	7.38	7.40	.12	.00	.41	57P PH, COLD, RADIOMETER TYPE PH M64			
L328	6	7.66	7.78	.58	.04	1.22	57M PH, COLD, BECKMAN ZEROMATIC			
L174C	6	7.74	7.78	.64	-.02	.89	57F PH, COLD, FISHER ACCUMET MODEL 220			
GMEANS:		7.31	7.31			1.00				
95% ELLIPSE:		2.20		.36			WITH GAMMA = 48 DEGREES			

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T57-2 TABLE 1  
 HYDROGEN ION CONCENTRATION (PH), HOT  
 TAPPI STANDARD T435 GS-77

JUNE 1978

LAB CODE	SAMPLE J77	PRINTING 89 GRAMS PER SQUARE METER				SAMPLE J14	PRINTING 89 GRAMS PER SQUARE METER				TEST D.O. = S		
		MEAN	DEV	N. DEV	SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F
L128	7.620	.128	.1.01	.084	1.58	7.840	.084	1.26	.055	.82	57L	G	L128
L162	7.752	.004	.03	.084	1.58	7.766	.010	.14	.113	1.69	57C	G	L162
L174H	7.920	.172	1.36	.045	.84	7.680	.076	-1.15	.045	.67	57G	G	L174H
L182H	7.700	-.048	-.38	.000	.00	7.740	-.016	-.25	.055	.82	57E	G	L182H
L334	8.631	.883	6.96	.148	2.79	8.763	1.006	15.18	.062	.92	57C	H	L334
L484B	7.440	-.308	-.2.43	.152	2.86	7.360	-.396	-.5.98	.089	1.34	57Z	H	L484B
GR. MEAN = 7.748 PH UNITS						GRAND MEAN = 7.756 PH UNITS					TEST DETERMINATIONS = 5		
SD MEANS = .127 PH UNITS						SD OF MEANS = .066 PH UNITS					4 LABS IN GRAND MEANS		
AVERAGE SDR = .053 PH UNITS											AVERAGE SDR = .067 PH UNITS		
TOTAL NUMBER OF LABORATORIES REPORTING = 6													
Best values: J77 7.8 pH units													
J14 7.8 pH units													

The following laboratories were omitted from the  
 grand means because of extreme test results: 334, 484B

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T57-2 TABLE 2  
 HYDROGEN ION CONCENTRATION (PH), HOT  
 TAPPI STANDARD T435 GS-77

JUNE 1978

LAB CODE	F	MEANS J77	MEANS J14	COORDINATES	AVG	PROPERTY==TEST INSTRUMENT==CONDITIONS
MAJOR	MINOR	R. SDR	VAR			
L484B #	7.440	7.360	-.100	-.492	2.10	57Z PH, HOT, BECKMAN MODEL H2
L128 G	7.620	7.840	-.152	.018	1.20	57L PH, HOT, L*N
L182H G	7.700	7.740	-.036	-.036	.41	57B PH, HOT, RADIOMETER TYPE PH M 28
L162 G	7.752	7.766	-.001	.010	1.64	57C PH, HOT, CORNING MODEL 12 RESEARCH METER
L174H G	7.920	7.680	.188	.008	.76	57G PH, HOT, FISHER ACCUMET MODEL 220
L334 #	8.631	8.763	.345	1.294	1.85	57C PH, HOT, CORNING MODEL 12 RESEARCH METER
GMEANS:	7.748	7.756			1.00	
95% ELLIPSE:	7.072	.186			WITH GAMMA ==26 DEGREES	

## ANALYSIS T60-1 TABLE 1

OPACITY (89% REFLECTANCE BACKING) IN PERCENT

TAPPI STANDARD T425 GS-75. OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) - B&amp;L TYPE

LAB CODE	SAMPLE E40	COATED DULL				SAMPLE J57	PRINTING				TEST D. = 10		
		MEAN	DEV	N.DEV	SDR		MEAN	DEV	N.DEV	SDR	R.SDR	VAR	F
L105	96.48	.32	1.04	.14	.66	93.56	.82	1.51	.25	.69	60H	Ø	L105
L108	96.08	.08	.24	.06	.30	92.73	.01	.03	.19	.53	60B	Ø	L108
L115	96.07	.09	.28	.40	1.88	93.08	.34	.62	.39	1.04	60B	Ø	L115
L118	96.36	.20	.65	.13	.60	93.22	.48	.88	.25	.68	60B	Ø	L118
L121	95.93	.23	.72	.18	.87	92.45	.29	.54	.51	1.37	60B	Ø	L121
L122	92.31	-3.85	-12.31	.15	.72	86.31	-6.43	-11.92	.26	.71	60D	#	L122
L123	96.20	.04	.14	.16	.74	92.64	.10	.19	.34	.93	60W	Ø	L123
L124	95.62	.54	-1.72	.47	2.21	92.12	.62	-1.16	.36	.98	60B	Ø	L124
L125	96.13	.03	.08	.22	1.05	92.80	.06	.10	.32	.85	60H	Ø	L125
L131	95.89	.27	.85	.22	1.06	92.06	.68	-1.27	.17	.46	60R	Ø	L131
L132	95.83	.33	-1.04	.08	.39	92.60	.14	.27	.53	1.42	60B	Ø	L132
L136	95.91	.25	.79	.10	.47	92.41	.33	.62	.32	.88	60H	Ø	L136
L139	96.08	.08	.24	.16	.77	92.90	.16	.29	.38	1.03	60B	Ø	L139
L148H	96.29	.13	.43	.15	.72	92.32	.42	.79	.38	1.02	60H	#	L148H
L152	96.34	.18	.59	.16	.78	93.06	.32	.58	.41	1.10	60B	Ø	L152
L153	96.45	.29	.94	.37	1.75	93.05	.31	.57	.44	1.18	60B	Ø	L153
L157	96.60	.44	1.42	.32	1.50	93.40	.66	1.21	.57	1.53	60B	Ø	L157
L158	96.49	.33	1.07	.16	.76	93.44	.70	1.29	.42	1.15	60D	Ø	L158
L159	96.34	.18	.59	.13	.60	92.76	.02	.03	.34	.91	60R	Ø	L159
L162	96.49	.33	1.07	.12	.57	93.30	.56	1.03	.47	1.27	60W	Ø	L162
L166	95.73	.43	-1.36	.13	.59	92.11	.63	-1.17	.44	1.18	60B	Ø	L166
L173A	96.47	.31	1.00	.12	.55	93.58	.84	1.55	.26	.70	60B	Ø	L173A
L182	95.85	.31	.98	.41	1.95	92.15	.59	-1.10	.24	.65	60B	Ø	L182
L190C	96.29	.13	.43	.15	.72	93.05	.31	.57	.27	.73	60B	Ø	L190C
L190R	96.24	.08	.27	.14	.68	92.73	.01	-.03	.21	.56	60B	Ø	L190R
L206	96.19	.03	.11	.12	.57	92.76	.02	.03	.23	.61	60B	Ø	L206
L210B	96.17	.01	.04	.08	.39	92.76	.02	.03	.31	.84	60B	Ø	L210B
L210D	96.20	.04	.14	.12	.55	92.72	.02	-.04	.36	.99	60D	Ø	L210D
L211S	96.02	.14	-.44	.23	1.09	92.94	.20	.36	.41	1.10	60R	Ø	L211S
L213	95.93	.23	-.72	.09	.45	92.44	.30	-.56	.39	1.05	60B	Ø	L213
L223B	96.52	.36	1.16	.11	.54	93.28	.54	.99	.31	.83	60B	Ø	L223B
L225	96.05	.11	.34	.33	1.57	92.44	.30	-.56	.64	1.73	60B	Ø	L225
L228	96.07	.09	.23	.16	.74	92.69	.05	-.10	.21	.56	60B	Ø	L228
L230	96.26	.10	.33	.13	.64	92.53	.21	-.40	.43	1.16	60B	Ø	L230
L233B	95.50	.66	-2.10	.71	3.35	92.20	.54	-1.01	.71	1.93	60B	#	L233B
L236B	95.46	.70	-2.23	.41	1.94	91.40	-1.34	-2.49	.00	.00	60B	Ø	L236B
L238A	95.50	.66	-2.10	.09	.45	91.62	-1.12	-2.08	.35	.93	60R	Ø	L238A
L241	96.03	.13	.40	.22	1.02	93.00	.26	.47	.32	.86	60B	Ø	L241
L243	96.19	.03	.11	.15	.72	92.62	.12	-.23	.42	1.15	60B	Ø	L243
L254	96.60	.44	1.42	.17	.80	93.62	.88	1.62	1.01	2.73	60H	Ø	L254
L255	95.99	.17	-.53	.13	.61	92.92	.18	.33	.41	1.11	60B	Ø	L255
L259	96.22	.06	.20	.19	.91	93.12	.38	.70	.38	1.03	60B	Ø	L259
L261	96.70	.54	1.74	.42	2.00	93.17	.43	.79	.25	.67	60B	Ø	L261
L262	95.85	.31	.98	.23	1.08	91.98	.76	-1.42	.15	.42	60B	Ø	L262
L275	96.04	.12	-.37	.13	.64	92.23	.51	-.95	.19	.53	60R	Ø	L275
L278	96.52	.36	1.16	.18	.83	93.38	.64	1.18	.28	.76	60B	Ø	L278
L281	96.32	.16	.52	.13	.62	93.06	.32	.58	.21	.57	60D	Ø	L281
L285B	95.86	.30	-.95	.26	1.23	92.24	.50	-.93	.44	1.20	60B	Ø	L285B
L285R	96.03	.13	-.40	.20	.95	91.95	.79	-1.47	.30	.81	60R	Ø	L285R
L288	96.09	.07	-.21	.03	.15	92.76	.02	-.03	.38	1.02	60D	Ø	L288
L301	95.95	.21	-.66	.10	.46	92.21	.53	-.99	.35	.95	60B	Ø	L301
L305	96.08	.08	-.24	.14	.66	92.60	.14	-.27	.16	.42	60R	Ø	L305
L308	96.33	.17	.56	.25	1.18	93.19	.45	.83	.38	1.01	60H	Ø	L308
L315	96.11	.05	-.15	.14	.69	92.50	.24	-.45	.27	.74	60D	Ø	L315
L317	96.24	.08	.27	.22	1.03	92.69	.05	-.10	.73	1.96	60B	Ø	L317
L318	96.30	.14	.46	.26	1.22	93.15	.41	.75	.24	.65	60B	Ø	L318
L323	97.04	.88	2.82	.35	1.66	93.85	1.11	2.05	.58	1.56	60W	#	L323
L326	96.51	.35	1.13	.54	2.56	93.07	.33	.60	.58	1.58	60B	Ø	L326
L328	95.90	.26	-.82	.32	1.50	92.40	.34	-.64	.70	1.89	60B	Ø	L328
L333	96.65	.49	1.58	.78	3.71	93.70	.96	1.77	.95	2.56	60B	Ø	L333
L339	96.25	.09	.30	.35	1.67	93.10	.36	.66	.52	1.40	60B	Ø	L339
L341	95.72	.44	-1.40	.22	1.04	91.74	-1.00	-1.86	.41	1.10	60R	Ø	L341
L349	96.43	.27	.88	.09	.45	93.24	.50	.92	.07	.19	60D	Ø	L349
L352	95.98	.18	-.56	.09	.44	92.40	.34	-.64	.27	.74	60R	Ø	L352
L354	95.90	.26	-.82	.32	1.50	92.20	.54	-1.01	.63	1.71	60B	Ø	L354

OPACITY (89% REFLECTANCE BACKING) IN PERCENT  
TAPPI STANDARD T425 OS=75. OPACITY OF PAPER (15 DSG./DIFFUSE, ILLUMINANT A) = B&L TYPE

LAB CODE	SAMPLE E40	COATED DULL				SAMPLE J57	PRINTING				TEST D. = 10			
		MEAN	DEV	N. DEV	SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L366	95.44	-.72	+2.29	.50	2.35	92.84	.10	.18	.45	1.22	60B	X	L366	
L390	96.40	.24	.78	.52	2.45	93.30	.56	1.03	.48	1.31	60B	G	L390	
L523	96.01	-.15	+.47	.07	.35	92.42	-.32	-.60	.27	.74	60R	G	L523	
L543	95.81	-.35	+1.11	.12	.57	92.05	-.69	+1.29	.26	.71	60D	G	L543	
L561	94.80	+.136	+4.34	.42	2.00	92.20	-.54	+1.01	.42	1.14	60B	X	L561	
L581	96.15	-.01	+.02	.14	.64	92.67	-.07	+.14	.33	.90	60B	G	L581	
L587	96.36	.20	.65	.17	.81	93.04	.30	.55	.22	.60	60B	G	L587	
L592	95.97	-.19	+.60	.13	.63	91.99	-.75	+1.40	.23	.62	60W	G	L592	
L594	95.78	-.38	+1.20	.14	.66	92.66	-.08	+.16	.26	.71	60D	G	L594	
L597	96.00	-.16	+.50	.47	2.23	92.30	-.44	+.82	.48	1.31	60B	G	L597	
L599	96.20	.04	.14	.35	1.66	93.15	.41	.75	.63	1.69	60B	G	L599	
L608	97.03	.87	2.80	+14	.67	94.10	1.36	2.51	.26	.71	60D	*	L608	
GR. MEAN =	96.16	PERCENT				GRAND MEAN =	92.74	PERCENT			TEST DETERMINATIONS =	10		
SD MEANS =	.31	PERCENT				SD OF MEANS =	.54	PERCENT			74 LABS IN GRAND MEANS			
AVERAGE SDR =	.21	PERCENT				AVERAGE SDR =	.37	PERCENT						
L224	95.65	-.51	+1.62	.41	1.95	91.40	-.134	+2.49	.32	.85	60P	*	L224	
L236E	96.73	.57	1.84	.11	.50	93.33	.59	1.08	.21	.56	60E	*	L236E	
L249	96.34	.18	.59	.07	.33	92.49	-.25	+.47	.35	.94	60P	*	L249	
L256	96.24	.09	.28	.12	.55	92.01	-.74	+1.36	.27	.73	60N	*	L256	
L260	96.50	.34	1.10	.41	1.93	92.60	-.14	+.27	.32	.85	60P	*	L260	
L309	95.23	-.93	+2.96	.16	.74	91.57	-.1.17	-2.17	.36	.97	60A	*	L309	
L312	95.85	-.31	-.98	.24	1.14	91.85	-.89	+1.66	.24	.65	60P	*	L312	
L314	96.53	.37	1.20	.13	.63	93.34	.60	1.10	.47	1.28	60T	*	L314	
L380	96.00	-.16	-.50	.00	.00	92.00	-.74	+1.38	.00	.00	60P	*	L380	
L388	95.60	-.56	+1.78	.32	1.50	91.45	-.1.29	-2.40	.50	1.34	60P	*	L388	
TOTAL NUMBER OF LABORATORIES REPORTING =	87													

Best values: E40 96.2 + 0.5 percent  
J57 92.7 + 0.9 percent

The following laboratories were omitted from the grand means because of extreme test results: 122

## ANALYSIS T60-1 TABLE 2

OPACITY (8% REFLECTANCE BACKING) IN PERCENT

TAPPI STANDARD T425 GS-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) = B&amp;L TYPE

LAB CODE	F	MEANS E40	COORDINATES J57	MAJOR MINOR	AVG E.S.DR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L122 #		92.31	86.31	-7.49	.31	.72 60D OPACITY (WHITE BACKING), DIANG/BNL
L561 X		94.80	92.20	-1.13	.93	1.57 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L309 *		95.23	91.57	-1.47	.25	.86 60A OPACITY (WHITE BACKING), ZEISS HLREPHG, FILTER 4,86% BACKING
L366 X		95.44	92.84	-.26	.68	1.79 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L236B #		95.46	91.40	-1.51	-.03	.97 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L238A #		95.50	91.62	-1.30	.04	.69 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L233B *		95.50	92.20	-.79	.32	2.64 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L3B8 *		95.60	91.45	-1.40	-.13	1.42 60P OPACITY (WHITE BACKING), PHOTOVGLT
L124 #		95.62	92.12	-.80	.17	1.59 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L224 *		95.65	91.40	-1.42	-.20	1.40 60P OPACITY (WHITE BACKING), PHOTOVGLT
L341 #		95.72	91.74	-1.09	-.10	1.07 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L166 #		95.73	92.11	-.76	.07	.89 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L594 #		95.78	92.66	-.25	.29	.69 60D OPACITY (WHITE BACKING), DIANG/BNL
L543 #		95.81	92.05	-.78	-.03	.64 60D OPACITY (WHITE BACKING), DIANG/BNL
L132 #		95.83	92.60	-.28	.22	.91 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L312 *		95.65	91.85	-.93	-.16	.90 60P OPACITY (WHITE BACKING), PHOTOVGLT
L262 #		95.85	91.98	-.82	-.10	.75 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L182 #		95.85	92.15	-.67	-.01	1.30 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L285B #		95.86	92.24	-.58	.02	1.21 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L131 #		95.89	92.06	-.73	-.09	.76 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L354 #		95.90	92.20	-.60	-.03	1.60 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L328 #		95.90	92.40	-.42	.06	1.69 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L136 #		95.91	92.41	-.41	.06	.67 60H OPACITY (WHITE BACKING), HUYGEN
L121 #		95.93	92.45	-.37	.06	1.12 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L213 #		95.93	92.44	-.38	.05	.75 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L301 #		95.95	92.21	-.57	-.07	.70 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L592 #		95.97	91.99	-.75	-.20	.63 60W OPACITY (WHITE BACKING), HUYGEN, DIGITAL
L352 #		95.98	92.40	-.39	-.01	.59 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L255 #		95.99	92.92	.08	.23	.86 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L380 *		96.00	92.00	-.73	-.22	.00 60P OPACITY (WHITE BACKING), PHOTOVGLT
L597 #		96.00	92.30	-.46	-.07	1.77 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L523 #		96.01	92.42	-.35	-.03	.55 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L211S #		96.02	92.94	.11	.21	1.10 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L285R #		96.03	91.95	-.76	-.27	.68 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L241 #		96.03	93.00	.16	.23	.94 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L275 #		96.04	92.23	-.51	-.14	.58 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L225 #		96.05	92.44	-.32	-.05	1.65 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L115 #		96.07	93.08	.25	.24	1.46 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L228 #		96.07	92.69	-.09	.05	.65 60H OPACITY (WHITE BACKING), HUYGEN
L139 #		96.08	92.90	.10	.14	.90 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L16B #		96.08	92.73	-.05	.06	.41 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L305 #		96.08	92.60	-.16	-.00	.54 60R OPACITY (WHITE BACKING), TWING-ALBERT (FORMERLY SRL)
L288 #		96.09	92.76	-.02	.07	.59 60D OPACITY (WHITE BACKING), DIANG/BNL
L315 #		96.11	92.50	-.24	-.08	.71 60D OPACITY (WHITE BACKING), DIANG/BNL
L125 #		96.13	92.80	.04	.05	.95 60H OPACITY (WHITE BACKING), HUYGEN
L581 #		96.15	92.67	-.07	-.03	.77 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L210B #		96.17	92.76	.02	-.00	.61 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L243 #		96.19	92.62	-.09	-.09	.93 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L206 #		96.19	92.76	.03	-.02	.59 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L123 #		96.20	92.64	-.07	-.09	.83 60W OPACITY (WHITE BACKING), HUYGEN, DIGITAL
L210D #		96.20	92.72	-.00	-.05	.77 60D OPACITY (WHITE BACKING), DIANG/BNL
L599 #		96.20	93.15	.38	.16	1.67 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L259 #		96.22	93.12	.36	.12	.97 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L190R #		96.24	92.73	.03	-.08	.62 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L317 #		96.24	92.69	-.01	-.10	1.50 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L256 *		96.24	92.01	-.60	-.43	.64 60N OPACITY (WHITE BACKING), HUNTER
L339 #		96.25	93.10	.36	.09	1.53 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L230 #		96.26	92.53	-.14	-.19	.90 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L190C #		96.29	93.05	.33	.03	.73 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L148H *		96.29	92.32	-.31	-.32	.87 60H OPACITY (WHITE BACKING), HUYGEN
L318 #		96.30	93.15	.43	.07	.94 60B OPACITY (WHITE BACKING), BAUSCH + LOMB
L281 #		96.32	93.06	.36	.01	.60 60D OPACITY (WHITE BACKING), DIANG/BNL
L308 #		96.33	93.19	.47	.06	1.10 60H OPACITY (WHITE BACKING), HUYGEN
L249 *		96.34	92.49	-.14	-.2B	.64 60P OPACITY (WHITE BACKING), PHOTOVGLT
L152 #		96.34	93.06	.37	-.01	.94 60B OPACITY (WHITE BACKING), BAUSCH + LOMB

## ANALYSIS T60-1 TABLE 2

OPACITY (89% REFLECTANCE BACKING) IN PERCENT


TAPPI STANDARD T425 OS-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) - B&amp;L TYPE

LAB CODE	MEANS F	E40	J57	COORDINATES MAJOR	MINOR	AVG R. SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L159	Ø	96.34	92.76	.10	-.15	.76 60R	OPACITY (WHITE BACKING), THWING-ALBERT (FORMERLY SRL)
L587	Ø	96.36	93.04	.36	-.04	.71 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L118	Ø	96.36	93.22	.52	.05	.64 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L390	Ø	96.40	93.30	.60	.05	1.88 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L349	Ø	96.43	93.24	.57	-.00	.32 60D	OPACITY (WHITE BACKING), DIANO/BNL
L153	Ø	96.45	93.05	.41	-.11	1.47 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L173A	Ø	96.47	93.58	.88	.12	.62 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L105	Ø	96.48	93.56	.87	.11	.68 60B	OPACITY (WHITE BACKING), HUYGEN
L162	Ø	96.49	93.30	.65	-.03	.92 60W	OPACITY (WHITE BACKING), HUYGEN, DIGITAL
L158	Ø	96.49	93.44	.77	.04	.95 60D	OPACITY (WHITE BACKING), DIANO/BNL
L260	*	96.50	92.60	.04	-.37	1.39 60P	OPACITY (WHITE BACKING), PHOTOVOLT
L326	Ø	96.51	93.07	.46	-.16	2.07 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L278	Ø	96.52	93.38	.73	-.02	.80 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L223B	Ø	96.52	93.28	.64	-.06	.69 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L314	*	96.53	93.34	.70	-.04	.95 60T	OPACITY (WHITE BACKING), SMALL SPHERE COLOR EYE
L157	Ø	96.60	93.40	.79	-.08	1.52 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L254	Ø	96.60	93.62	.98	.03	1.77 60H	OPACITY (WHITE BACKING), HUYGEN
L333	Ø	96.65	93.70	1.08	.02	3.14 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L261	Ø	96.70	93.17	.63	-.27	1.34 60B	OPACITY (WHITE BACKING), BAUSCH + LOEB
L236E	*	96.73	93.33	.79	-.22	.53 60E	OPACITY (WHITE BACKING), ZEISS SLREPHG, FMY-C(10) FILTER
L608	*	97.03	94.10	1.61	-.12	.69 60D	OPACITY (WHITE BACKING), DIANO/BNL
L323	*	97.04	93.85	1.39	-.25	1.61 60W	OPACITY (WHITE BACKING), HUYGEN, DIGITAL
GMEANS:		96.16	92.74			1.00	
95% ELLIPSE:				1.54	.32	WITH GAMMA = 61 DEGREES	

OPACITY, B&L TYPE, 89% BACKING

SAMPLE E40 = 96.16 PERCENT

SAMPLE J57 = 92.74 PERCENT

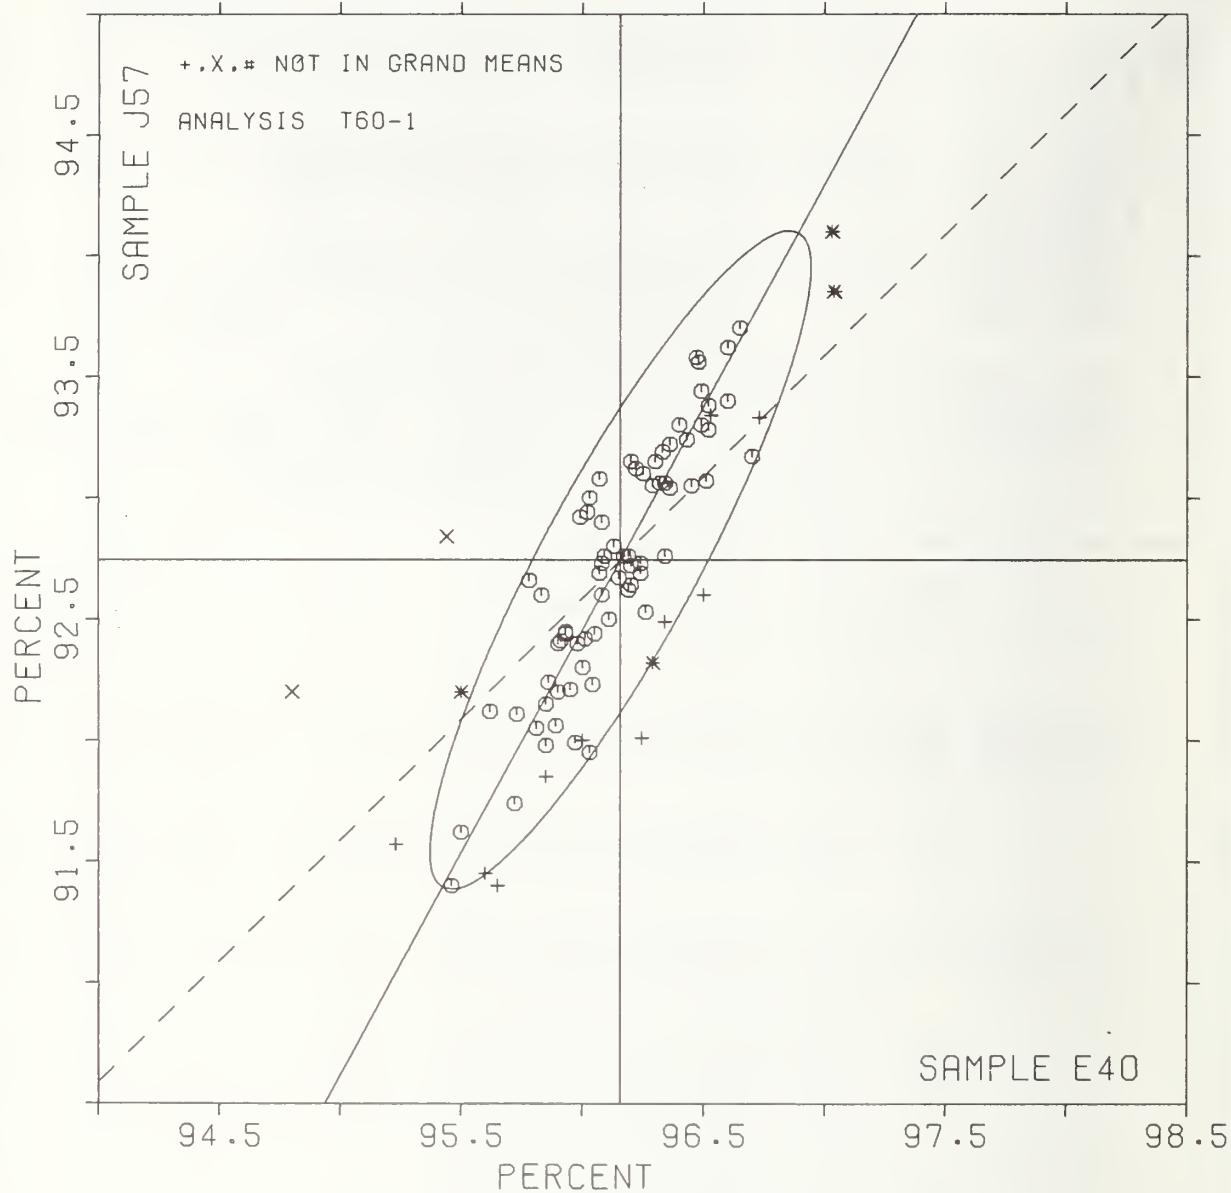

ANALYSIS T60-2 TABLE 1  
 OPACITY (PAPER BACKING) IN PERCENT

TAPPI STANDARD T425 GS-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) = B&amp;L TYPE

LAB CODE	SAMPLE E40 COATED DULL					SAMPLE J57 PRINTING					TEST D. = 10		
	MEAN	DEV	N. DEV	SDR	R.SDR	MEAN	DEV	N. DEV	SDR	R.SDR	VAR	F	LAB
L115	95.99	.08	.51	.34	1.40	93.07	.10	.29	.29	.99	60C	0	L115
L118	96.24	.17	1.12	.13	.52	93.38	.41	1.21	.21	.72	60C	0	L118
L190C	96.06	-.01	-.06	.14	.59	92.66	-.31	-.92	.45	1.52	60C	0	L190C
L190R	96.21	.14	.92	.13	.53	93.32	.35	1.03	.16	.54	60C	0	L190R
L236B	96.10	.03	.21	.32	1.31	92.60	-.37	-1.10	.39	1.30	60C	0	L236B
L243	96.10	.03	.21	.49	2.04	93.15	.18	.53	.36	1.22	60C	0	L243
L543	95.78	-.29	-1.88	.15	.61	92.62	-.35	-1.04	.21	.70	60V	0	L543
GR. MEAN = 96.07 PERCENT		GRAND MEAN = 92.97 PERCENT		TEST DETERMINATIONS = 10 7 LABS IN GRAND MEANS									
SD MEANS = .15 PERCENT		SD GP MEANS = .34 PERCENT		AVERAGE SDR = .24 PERCENT									
TOTAL NUMBER OF LABORATORIES REPORTING = 7		AVERAGE SDR = .30 PERCENT											

Best values: E40 96.1 percent  
 J57 93.0 percent

## OPACITY (PAPER BACKING) IN PERCENT

TAPPI STANDARD T425 GS-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) = B&amp;L TYPE

LAB CODE	MEANS		COORDINATES		AVG R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS		
	E40	J57	MAJOR	MINOR				
L543	0	95.78	92.62	-.43	.16	.66	60V	OPACITY (PAPER BACKING), DIANG/BNL
L115	0	95.99	93.07	.07	.11	1.19	60C	OPACITY (PAPER BACKING), BAUSCH + LGMB
L190C	0	96.06	92.66	-.30	-.09	1.05	60C	OPACITY (PAPER BACKING), BAUSCH + LGMB
L243	0	96.10	93.15	.18	.03	1.63	60C	OPACITY (PAPER BACKING), BAUSCH + LGMB
L236B	0	96.10	92.60	-.34	-.15	1.31	60C	OPACITY (PAPER BACKING), BAUSCH + LGMB
L190R	0	96.21	93.32	.38	-.02	.54	60C	OPACITY (PAPER BACKING), BAUSCH + LGMB
L118	0	96.24	93.38	.44	-.03	.62	60C	OPACITY (PAPER BACKING), BAUSCH + LGMB
GMEANS: 96.07 92.97		1.00		WITH GAMMA = 71 DEGREES				
95% ELLIPSE: 1.33 .40								

## ANALYSIS T60-3 TABLE 1

OPACITY (PAPER BACKING) IN PERCENT

TAPPI SUGGESTED METHOD TS19 GS-78, DIFFUSE OPACITY OF PAPER = ILLUMINANT C, ELREPHO TYPE

LAB CODE	SAMPLE E40	COATED DULL				SAMPLE J57	PRINTING				TEST D. = 10		
		MEAN	DEV	N. DEV	SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F
L182E	96.68	.01	.14	.08	.78	93.73	.18	1.03	.19	1.06	60J	G	L182E
L233P	96.75	.06	.55	.10	.97	93.54	.01	.05	.15	.82	60F	G	L233F
L244	96.52	.17	1.72	.11	1.13	93.24	.31	1.75	.19	1.04	60F	G	L244
L250T	96.74	.05	.45	.12	1.17	93.66	.11	.63	.24	1.29	60J	G	L250T
L251	96.69	.00	.02	.11	1.07	93.43	.12	.69	.22	1.22	60F	G	L251
L360	96.58	.11	1.13	.12	1.22	93.43	.12	.67	.21	1.15	60F	G	L360
L446	96.76	.07	.67	.08	.79	93.60	.05	.28	.10	.54	60J	G	L446
L575	96.83	.14	1.34	.09	.87	93.76	.22	1.22	.16	.88	60J	G	L575
GR. MEAN = 96.69 PERCENT						GRAND MEAN = 93.55 PERCENT					TEST DETERMINATIONS = 10		
SD MEANS = .10 PERCENT						SD OF MEANS = .18 PERCENT					8 LABS IN GRAND MEANS		
AVERAGE SDR = .10 PERCENT						AVERAGE SDR = .18 PERCENT							
L176 82.87 -13.82 -136.08		.21	2.05	83.73	-9.82	+55.59	.05	.26	60Z	* L176			
L626 96.77 .08 .74		.19	1.94	92.97	.58	=3.28	.14	.77	60Q	* L626			
TOTAL NUMBER OF LABORATORIES REPORTING = 10													

Best values: E40 96.7 percent  
J57 93.6 percent

## ANALYSIS T60-3 TABLE 2

OPACITY (PAPER BACKING) IN PERCENT

TAPPI SUGGESTED METHOD TS19 GS-78, DIFFUSE OPACITY OF PAPER = ILLUMINANT C, ELREPHO TYPE

LAB CODE	F	MEANS		COORDINATES		AVG	R. SDR	VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS		
		E40	J57	MAJOR	MINOR						
L176	*	82.87	83.73	-15.06	7.80	1.15	60Z	OPACITY (PAPER BACKING), MARTIN SWEETS			
L244	G	96.52	93.24	.35	.01	1.08	60F	OPACITY (PAPER BACKING), ZEISS ELREPHO, PMY-C(10) NO TRAP			
L350	G	96.58	93.43	.16	.05	1.19	60P	OPACITY (PAPER BACKING), ZEISS ELREPHO, FMY-C(10) NO TRAP			
L182E	G	96.68	93.73	.15	.10	.92	60J	OPACITY (PAPER BACKING), ZEISS ELREPHO, FMY-C(10) FILTER			
L251	G	96.69	93.43	.11	.05	1.14	60F	OPACITY (PAPER BACKING), ZEISS ELREPHO, PMY-C(10) NO TRAP			
L250T	G	96.74	93.66	.12	.01	1.23	60J	OPACITY (PAPER BACKING), ZEISS ELREPHO, FMY-C(10) FILTER			
L233F	G	96.75	93.54	.02	.05	.89	60P	OPACITY (PAPER BACKING), ZEISS ELREPHO, FMY-C(10) NO TRAP			
L446	G	96.76	93.60	.08	.04	.66	60J	OPACITY (PAPER BACKING), ZEISS ELREPHO, FMY-C(10) FILTER			
L626	*	96.77	92.97	.48	.33	1.35	60Q	OPACITY (PAPER BACKING), PHOTOVOLT			
L575	G	96.83	93.76	.25	.02	.88	60J	OPACITY (PAPER BACKING), ZEISS ELREPHO, FMY-C(10) FILTER			
GMEANS:		96.69	93.55			1.00					
95% ELLIPSE:		.68	.18			WITH GAMMA = 62 DEGREES					

ANALYSIS T65-1 TABLE 1  
 DIRECTIONAL BLUE REFLECTANCE IN PERCENT

TAPPI STANDARD T452 GS=77. 'BRIGHTNESS'; MARTIN SWEETS (ACST &amp; GE) IS STANDARD FOR THIS ANALYSIS

LAB CODE	SAMPLE J37	PRINTING 89 GRAMS PER SQUARE METER				SAMPLE J35	PRINTING 94 GRAMS PER SQUARE METER				TEST D. = 8		
		MEAN	DEV	N. DEV	SDR		MEAN	DEV	N. DEV	SDR	R.SDR	VAR	F
L108	75.59	=.20	.48	.04	.22	84.07	.10	.22	.18	1.30	65M	0	L108
L122	76.06	.27	.65	.16	1.01	83.81	=.16	=.37	.08	.59	65N	0	L122
L132	75.76	=.03	.07	.09	.58	83.66	=.31	=.71	.09	.65	65N	0	L132
L158	76.22	.43	1.03	.32	1.99	84.40	.42	.95	.33	2.37	65N	0	L158
L176A	72.72	=3.07	-7.30	.13	.81	79.66	=4.31	=9.72	.27	1.90	65A	#	L176A
L190C	75.06	=.73	-1.73	.12	.75	83.95	=.03	=.06	.08	.54	65A	0	L190C
L210M	76.04	.25	.59	.12	.75	83.81	=.16	=.37	.11	.80	65M	0	L210M
L210N	75.55	=.24	=.57	.12	.76	85.09	1.11	2.50	3.56	25.29	65N	#	L210N
L211	75.34	=.45	-1.08	.16	1.01	82.84	=1.14	=2.57	.40	2.84	65N	0	L211
L225	76.56	.77	1.84	.27	1.69	84.14	.16	.36	.18	1.31	65N	0	L225
L243	75.24	=.55	-1.32	.11	.67	83.59	=.39	=.88	.04	.25	65A	0	L243
L259	75.64	=.15	.36	.17	1.07	83.91	=.06	=.15	.12	.89	65M	0	L259
L275	75.61	=.18	=.42	.16	.98	83.74	=.24	=.54	.07	.53	65M	0	L275
L285	76.14	.35	.83	.17	1.07	84.65	.67	1.51	.23	1.61	65N	0	L285
L288	75.54	=.25	=.60	.18	1.12	83.84	=.14	=.32	.07	.53	65N	0	L288
L308	75.91	.12	.29	.11	.71	84.29	.31	.70	.10	.70	65N	0	L308
L315	75.60	=.19	=.45	.35	2.24	83.94	=.04	=.09	.07	.53	65N	0	L315
L317	75.29	=.50	-1.20	.22	1.41	83.86	=.11	=.26	.12	.84	65M	0	L317
L523	76.31	.52	1.24	.10	.63	84.11	.14	.30	.06	.46	65N	0	L523
L543	76.47	.68	1.63	.07	.45	83.81	=.16	=.37	.19	1.34	65M	0	L543
LS65	75.87	.08	.20	.10	.65	84.04	.06	.14	.13	.92	65A	0	LS65
LS98	76.69	.90	2.14	.35	2.20	86.02	2.05	4.61	.38	2.70	65M	#	LS98
GR. MEAN = 75.79 PERCENT		GRAND MEAN = 83.98 PERCENT				TEST DETERMINATIONS = 8							
SD MEANS = .42 PERCENT		SD OF MEANS = .44 PERCENT				20 LABS IN GRAND MEANS							
	AVERAGE	SDR	=	.16	PERCENT		AVERAGE	SDR	=	.14	PERCENT		
L105	75.77	=.02	=.04	.18	1.16	84.65	.67	1.51	.05	.38	65T	#	L105
L176I	75.91	.12	.29	.16	.98	84.99	1.01	2.27	.06	.46	65I	#	L176I
L213	76.06	.27	.65	.11	.67	84.62	.65	1.46	.07	.50	65T	#	L213
L223	76.87	1.08	2.58	.18	1.11	85.89	1.91	4.30	.10	.70	65G	#	L223
L241	76.54	.75	1.73	.20	1.26	85.52	1.55	3.49	.10	.74	65I	#	L241
L249	77.12	1.33	3.18	.09	.56	84.22	.25	.56	.09	.63	65P	#	L249
L256	75.74	=.05	=.13	.21	1.31	83.94	=.04	=.09	.11	.75	65H	#	L256
L260	76.14	.35	.83	.13	.82	84.19	.21	.47	.12	.89	65P	#	L260
L278	78.12	2.33	5.56	.23	1.46	86.12	2.15	4.84	.23	1.64	65P	#	L278
L301	76.40	.61	1.45	.18	1.12	84.37	.40	.90	.09	.63	65G	#	L301
L312	78.00	2.21	5.26	.27	1.69	84.37	.40	.90	.44	3.15	65P	#	L312
L321	78.81	3.02	7.19	.26	1.64	86.81	2.84	6.39	.59	4.22	65P	#	L321
L328	76.95	1.16	2.76	.09	.59	83.85	=.13	=.29	.11	.76	65P	#	L328
L339	76.37	.58	1.39	.23	1.46	83.12	=.85	=1.92	.19	1.34	65P	#	L339
L380	78.87	3.08	7.34	.35	2.24	84.62	.65	1.46	.52	3.68	65P	#	L380
L388	75.50	=.29	=.69	.00	.00	83.75	=.23	=.51	.27	1.90	65P	#	L388
LS62	81.00	5.21	12.40	.00	.00	86.00	2.02	4.56	.00	.00	65P	#	LS62
LS87	76.07	.28	.68	.10	.65	84.66	.69	1.54	.13	.92	65I	#	LS87
LS91	74.96	=.83	-1.98	.17	1.05	84.13	.15	.34	.10	.73	65H	#	L591
L626	77.97	2.18	5.20	.05	.29	86.12	2.15	4.84	.07	.50	65P	#	L626
TOTAL NUMBER OF LABORATORIES REPORTING = 42													

Best values: J37 75.6 + 0.8 percent  
 J35 83.8 + 0.9 percent


The following laboratories were omitted from the grand means because of extreme test results: 176A, 598

LAB CODE	F	MEANS J37	J35	COORDINATES MAJOR	MINOR	AVG R. SDR VAR	PROPERTY--TEST INSTRUMENT--CONDITIONS
L176A #	72.72	79.66	=5.28	=.41	1.35	65A BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (ACBT), S=2	
L591 #	74.96	84.13	=.42	.73	.89	65H BLUE REFLECTANCE (DIRECTIONAL), HUNTER	
L190C #	75.06	83.95	=.49	.54	.64	65A BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (ACBT), S=2	
L243 #	75.24	83.59	=.65	.17	.46	65A BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (ACBT), S=2	
L317 #	75.29	83.86	=.41	.31	1.13	65M BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (GE), S=1	
L211 #	75.34	82.84	=1.17	=.38	1.92	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L388 #	75.50	83.75	=.36	.08	.95	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L288 #	75.54	83.84	=.27	.10	.82	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L210N *	75.55	85.09	.70	.90	13.02	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L108 #	75.59	84.07	=.06	.22	.76	65M BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (GE), S=1	
L315 #	75.60	83.94	=.15	.12	1.39	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L275 #	75.61	83.74	=.30	=.02	.76	65M BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (GE), S=1	
L259 #	75.64	83.91	=.15	.08	.98	65M BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (GE), S=1	
L256 #	75.74	83.94	=.06	.02	1.03	65H BLUE REFLECTANCE (DIRECTIONAL), HUNTER	
L132 #	75.76	83.66	=.26	=.18	.61	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L105 #	75.77	84.65	.51	.44	.77	65T BLUE REFLECTANCE (DIRECTIONAL), HUNTER D25D2M	
L565 #	75.87	84.04	.10	=.03	.79	65A BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (ACBT), S=2	
L176I #	75.91	84.99	.85	.55	.72	65I BLUE REFLECTANCE (DIRECTIONAL), HUNTER D25D2A	
L308 #	75.91	84.29	.32	.11	.71	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L210M #	76.04	83.81	.03	=.30	.78	65M BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (GE), S=1	
L122 #	76.06	83.81	.05	=.31	.80	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L213 #	76.06	84.62	.67	.21	.59	65T BLUE REFLECTANCE (DIRECTIONAL), HUNTER D25D2M	
L587 #	76.07	84.66	.71	.22	.79	65I BLUE REFLECTANCE (DIRECTIONAL), HUNTER D25D2A	
L260 #	76.14	84.19	.38	.13	.85	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L285 #	76.14	84.65	.74	.16	1.34	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L158 #	76.22	84.40	.60	=.06	2.18	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L523 #	76.31	84.11	.44	=.31	.54	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L339 #	76.37	83.12	=.28	=.99	1.40	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L301 #	76.40	84.37	.70	.21	.88	65G BLUE REFLECTANCE (DIRECTIONAL), GARDNER	
L543 #	76.47	83.81	.31	=.63	.89	65M BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (GE), S=1	
L241 #	76.54	85.52	1.67	.42	1.00	65I BLUE REFLECTANCE (DIRECTIONAL), HUNTER D25D2A	
L225 #	76.56	84.14	.62	=.49	1.50	65N BLUE REFLECTANCE (DIRECTIONAL), DIANG/MARTIN SWEETS, S=4	
L598 #	76.69	86.02	2.15	.62	2.45	65M BLUE REFLECTANCE (DIRECTIONAL), MARTIN SWEETS (GE), S=1	
L223 #	76.87	85.89	2.16	.39	.91	65G BLUE REFLECTANCE (DIRECTIONAL), GARDNER	
L328 #	76.95	83.85	.65	=.97	.67	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L249 #	77.12	84.22	1.05	=.87	.59	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L626 #	77.97	86.12	3.05	=.30	.40	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L312 #	78.00	84.37	1.72	=1.44	2.42	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L278 #	78.12	86.12	3.14	=.42	1.55	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L321 #	78.81	86.81	4.11	=.50	2.93	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L380 #	78.87	84.62	2.47	=1.95	2.96	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
L562 #	81.00	86.00	4.89	=2.70	.00	65P BLUE REFLECTANCE (DIRECTIONAL), PHOTOVOLT	
GMEANS:	75.79	83.98		1.00			
95% ELLIPSE:	1.36	.98		WITH GAMMA = 50 DEGREES			

## BLUE REFLECTANCE, DIRECTIONAL

SAMPLE J37 = 75.8 PERCENT

SAMPLE J35 = 84.0 PERCENT

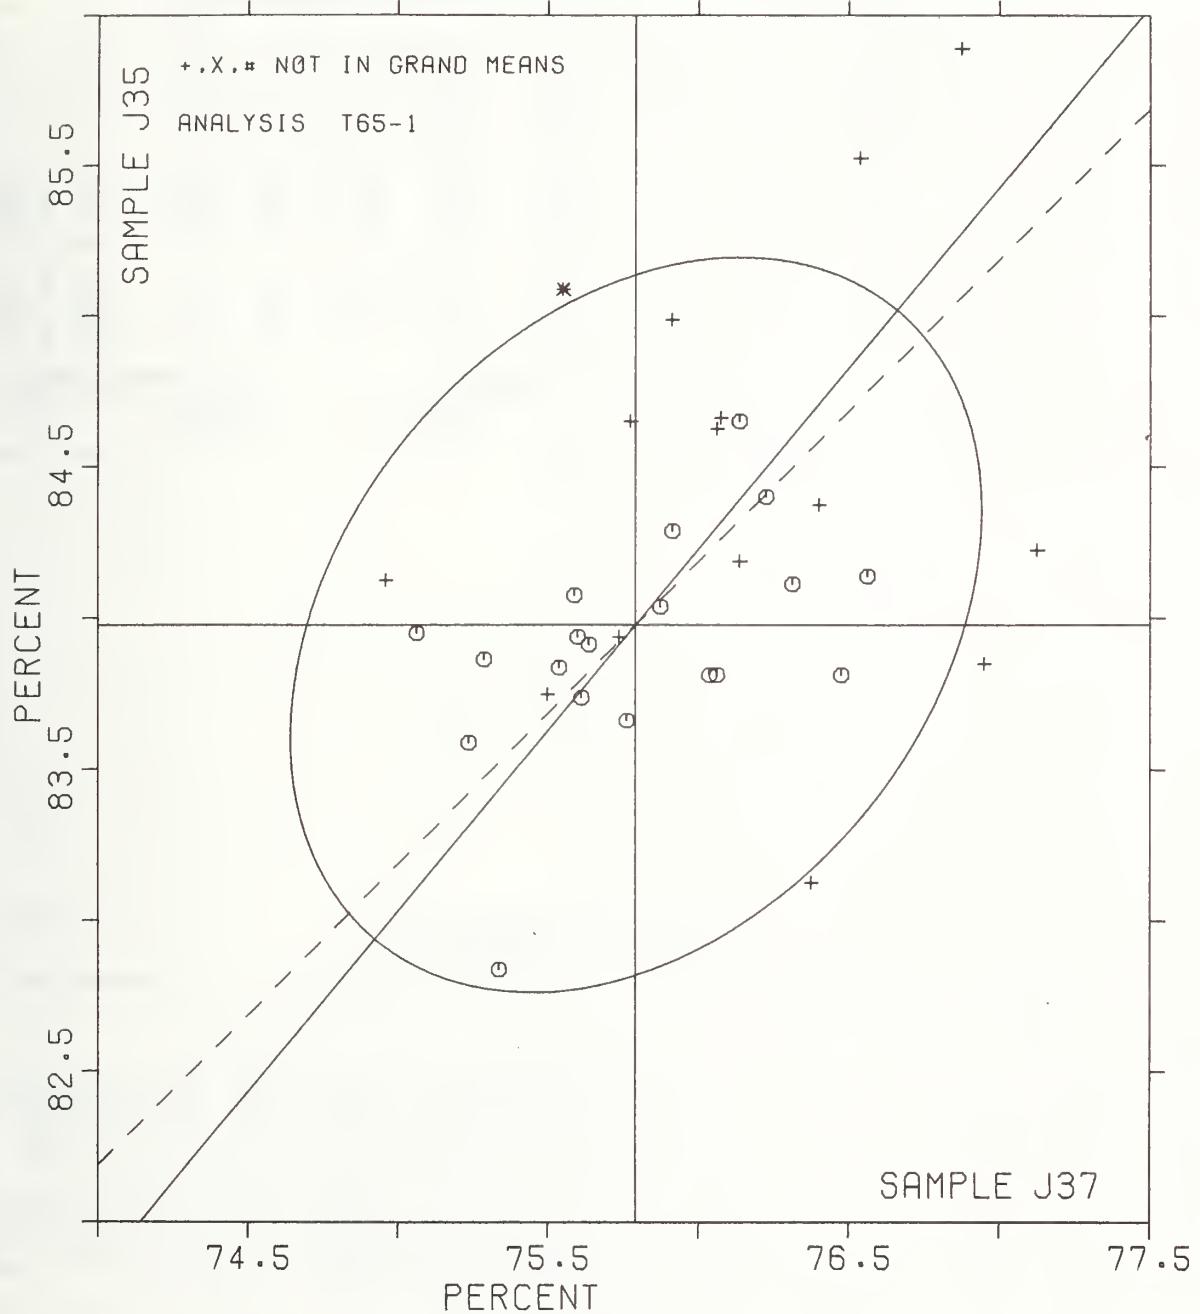

## ANALYSIS T65-2 TABLE 1

DIFFUSE BLUE REFLECTANCE IN PERCENT (GLOSS TRAP)

TAPPI SUGGESTED METHOD TS25 SU-72, BRIGHTNESS OF PULP (DIFFUSE ILLUMINATION AND 0 DEG. OBSERVATION)

LAB CODE	SAMPLE J37					SAMPLE J35					PRINTING TEST D. = 8				
	MEAN	89 GRAMS PER SQUARE METER	PRINTING DEV	N. DEV	SDR	MEAN	94 GRAMS PER SQUARE METER	PRINTING DEV	N. DEV	SDR	R. SDR	VAR	F	LAB	
L121	75.19	.24	.82	.30	.205	84.40	.03	.22	.08	.90	.65K	6	L121		
L136	75.88	.45	1.53	.12	.80	84.68	.25	1.75	.17	1.67	.65P	6	L136		
L170	75.10	.33	-1.12	.05	.36	84.20	.23	-1.61	.00	.00	.65B	6	L170		
L182	75.45	.02	.06	.19	1.26	84.46	.03	.20	.11	1.15	.65P	6	L182		
L210K	76.70	1.27	4.32	.16	1.09	85.41	.98	6.94	.07	.76	.65K	#	L210K		
L236	75.18	.25	.87	.11	.73	84.41	.02	.13	.07	.76	.65K	6	L236		
L250T	75.79	.36	1.22	.11	.73	84.48	.05	.38	.17	1.63	.65F	6	L250T		
L280	75.77	.34	1.17	.18	1.21	84.48	.05	.36	.11	1.23	.65Q	6	L280		
L325	76.42	.99	3.38	.15	1.01	85.61	1.18	8.33	.13	1.40	.65P	#	L325		
L349	76.06	.63	2.17	.14	.93	85.45	1.02	7.21	.05	.56	.65K	#	L349		
L362	74.46	.97	-3.30	.12	.85	83.36	-1.07	-7.56	.07	.76	.65K	#	L362		
L446	75.17	.26	.88	.14	.95	84.28	-.15	-1.05	.10	1.03	.65P	6	L446		
L575	75.49	.07	.22	.12	.81	84.32	-.11	-.79	.04	.40	.65F	6	L575		
L636	75.28	-.15	-.52	.16	1.10	84.58	.16	1.11	.08	.81	.65K	6	L636		
GR. MEAN = 75.43 PERCENT						GRAND MEAN = 84.43 PERCENT					TEST DETERMINATIONS = 8				
SD MEANS = .29 PERCENT						SD GP MEANS = .14 PERCENT					10 LABS IN GRAND MEANS				
AVERAGE SDR = .15 PERCENT						AVERAGE SDR = .09 PERCENT									
L289 75.41 -.02 -.05 .08 .57						84.35 -.08 -.55 .05 .58					656	*	L289		
TOTAL NUMBER OF LABORATORIES REPORTING = 15															

Best values: J37 75.4 percent  
J35 84.4 percentThe following laboratories were omitted from the  
grand means because of extreme test results: 210K,  
325, 349, 362

## ANALYSIS T65-2 TABLE 2

DIFFUSE BLUE REFLECTANCE IN PERCENT (GLOSS TRAP)


TAPPI SUGGESTED METHOD TS25 SU-72, BRIGHTNESS OF PULP (DIFFUSE ILLUMINATION AND 0 DEG. OBSERVATION)

LAB CODE	P	MEANS J37	MEANS J35	COORDINATES	AVG	PROPERTY---TEST INSTRUMENT---CONDITIONS
LAB CODE	P	J37	J35	MAJOR	MINOR	R. SDR VAR
L362	#	74.46	83.36	-1.27	.68	.81 65K DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, MG6 (ZBISS) BASE
L170	6	75.10	84.20	-.39	-.10	.18 65B DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, NBS ABSOLUTE BASE
L446	6	75.17	84.28	-.29	-.05	.99 65F DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, NRC-PTB ABSOLUTE BASE
L236	6	75.18	84.41	-.24	.07	.75 65K DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, MG6 (ZBISS) BASE
L211	6	75.19	84.40	-.24	.05	1.47 65K DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, MG6 (ZBISS) BASE
L636	6	75.28	84.58	-.09	.20	.96 65K DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, MG6 (ZBISS) BASE
L289	*	75.41	84.35	-.04	-.07	.57 65D DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, SPECIFIC CALIBRATION
L182	6	75.45	84.46	.03	.02	1.21 65P DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, NRC-PTB ABSOLUTE BASE
L575	6	75.49	84.32	.02	-.13	.60 65F DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, NRC-PTB ABSOLUTE BASE
L280	6	75.77	84.48	.34	-.07	1.22 65Q DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, ZBISS ABSOLUTE BASE
L250T	6	75.79	84.48	.36	-.07	1.28 65P DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, NRC-PTB ABSOLUTE BASE
L136	6	75.88	84.68	.51	.08	1.34 65F DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, NRC-PTB ABSOLUTE BASE
L349	#	76.06	85.45	.94	.75	.74 65K DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, MG6 (ZBISS) BASE
L325	#	76.42	85.61	1.33	.78	1.20 65P DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, NRC-PTB ABSOLUTE BASE
L210K	#	76.70	85.41	1.52	.50	.93 65K DIFFUSE REFLECTANCE, ELREPHG, GL.TRAP, MG6 (ZBISS) BASE
GMBANS: 75.45 84.43				1.00		
95% ELLIPSE:				.98	.32	WITH GAMMA = 19 DEGREES

BLUE REFLECTANCE, DIFFUSE, WITH TRAP

SAMPLE J37 = 75.43 PERCENT

SAMPLE J35 = 84.43 PERCENT

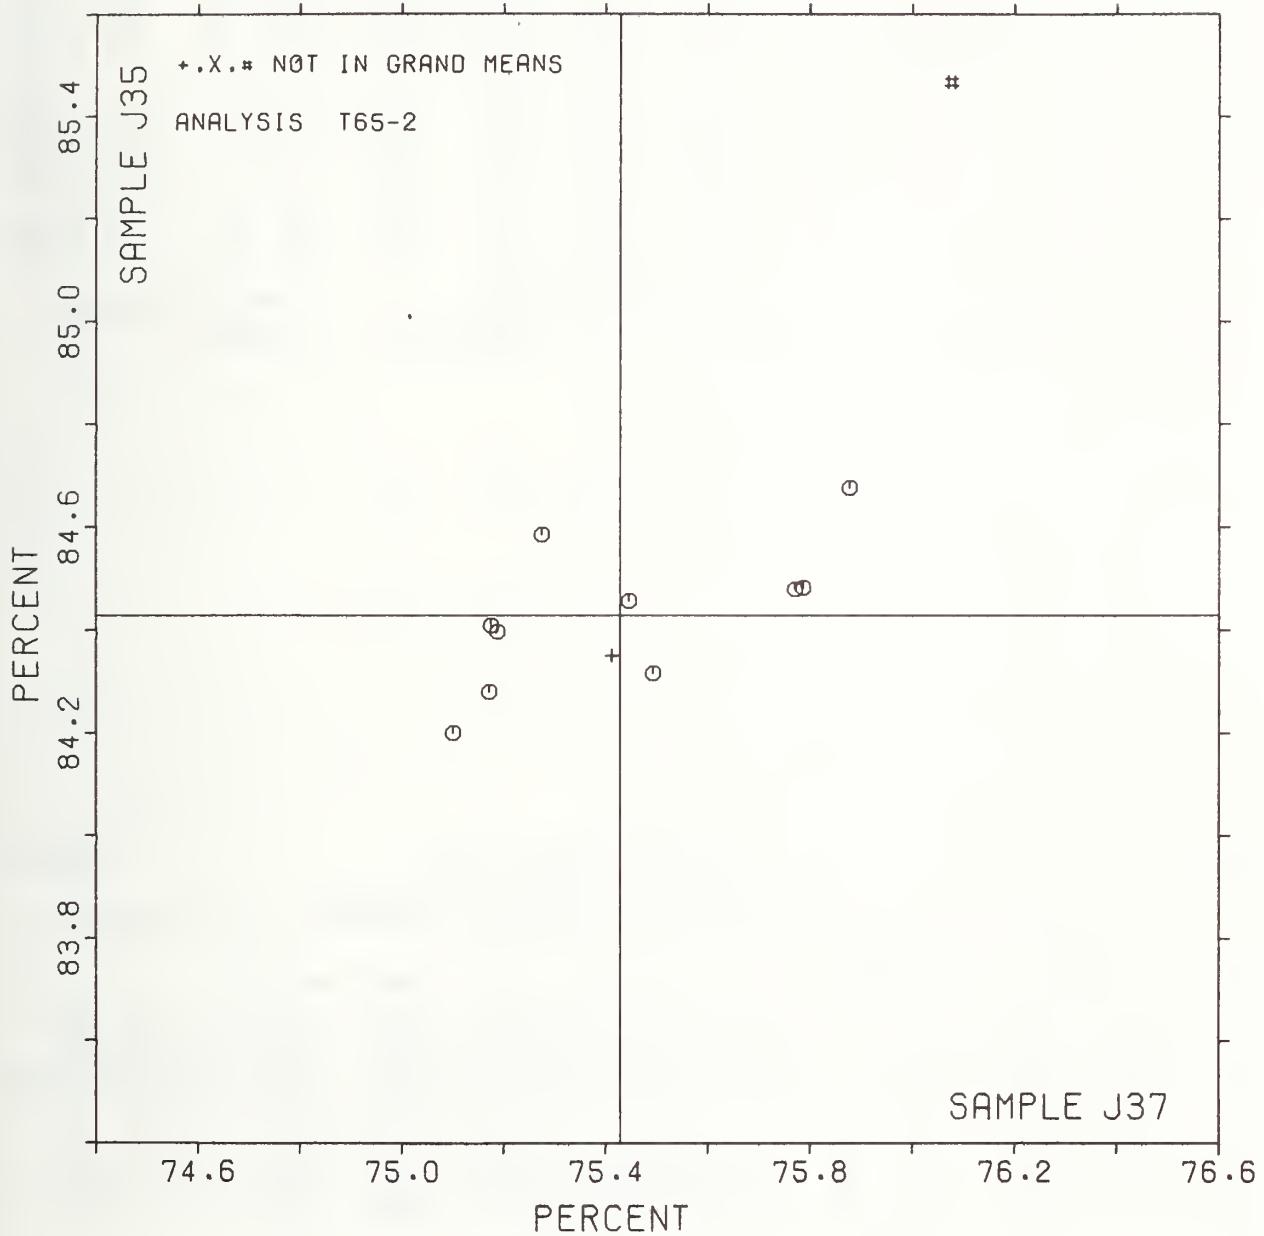

## ANALYSIS T65-3 TABLE 1

DIFFUSE BLUE REFLECTANCE IN PERCENT (NO GLOSS TRAP)

TAPPI SUGGESTED METHOD T525 SU-72, BRIGHTNESS OF PULP (DIFFUSE ILLUMINATION AND 0 DEG. OBSERVATION)

LAB CODE	SAMPLE J37	PRINTING 89 GRAMS PER SQUARE METER				SAMPLE J35	PRINTING 94 GRAMS PER SQUARE METER				TEST D. = 8 VAR F LAB
		MEAN	DEV	N.DEV	SDR		MEAN	DEV	N.DEV	SDR	
L115	74.97	+1.61	-4.33	.13	1.18	82.64	+1.64	-5.01	.06	1.10	65E # L115
L152	76.49	-0.09	+0.24	.13	1.15	82.90	+1.37	-4.21	.05	.92	65E # L152
L157	76.56	-0.03	+0.07	.10	.89	83.90	+0.38	-1.16	.05	.92	65E # L157
L161	77.02	+0.43	1.17	.11	1.01	84.37	.09	.29	.05	.86	65E # L161
L173A	76.68	+0.10	+0.26	.14	1.22	84.66	.38	1.17	.04	.61	65E # L173A
L194	75.80	+0.79	+2.12	.05	.42	83.65	+0.63	+1.92	.00	.00	65E # L194
L238A	76.87	+0.28	.76	.08	.68	84.27	+0.00	-.01	.07	1.22	65E # L238A
L244	76.85	+0.26	.70	.11	1.04	84.72	.44	1.35	.08	1.31	65D # L244
L251	76.52	-0.06	+0.17	.09	.83	84.10	+0.18	+0.55	.05	.92	65E # L251
L255	78.16	1.57	4.23	.16	1.48	86.04	1.77	5.41	.05	.91	65D # L255
L360	76.92	.33	.90	.21	1.86	84.47	.20	.60	.10	1.78	65E # L360
L384	76.41	-0.17	+0.46	.16	1.40	84.29	.01	.04	.06	1.11	65S # L384
L565	76.22	+0.36	+0.97	.07	.64	84.34	.06	.19	.07	1.28	65W # L565

GR. MEAN = 76.58 PERCENT

SD MEANS = .37 PERCENT

GRAND MEAN = 84.28 PERCENT

SD OF MEANS = .33 PERCENT

TEST DETERMINATIONS = 8

AVERAGE SDR = .11 PERCENT

AVERAGE SDR = .06 PERCENT

10 LABS IN GRAND MEANS

TOTAL NUMBER OF LABORATORIES REPORTING = 13

Best values: J37 76.5 percent

J35 84.3 percent

The following laboratories were omitted from the grand means because of extreme test results: 115,  
152, 255

## ANALYSIS T65-3 TABLE 2

DIFFUSE BLUE REFLECTANCE IN PERCENT (NO GLOSS TRAP)

TAPPI SUGGESTED METHOD T525 SU-72, BRIGHTNESS OF PULP (DIFFUSE ILLUMINATION AND 0 DEG. OBSERVATION)


LAB CODE	F	MEANS J37	MEANS J35	COORDINATES	AVG	PROPERTY---TEST INSTRUMENT---CONDITIONS
MAJOR	MINOR	R.SDR	VAR			
L115	#	74.97	82.64	+2.28	-.23	1.14 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L194	6	75.80	83.65	+1.01	.02	.21 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L565	6	76.22	84.34	-.24	.28	.96 65W DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, NBS MGG BASE
L384	6	76.41	84.29	-.12	.12	1.25 65S DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, ABSOLUTE-UNKNOWN BASE
L152	#	76.49	82.90	-.95	+1.00	1.04 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L251	6	76.52	84.10	-.16	-.10	.88 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L157	6	76.56	83.90	+.26	.27	.91 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L173A	6	76.68	84.66	.32	.23	.91 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L244	6	76.85	84.72	.48	.17	1.17 65D DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, NRC-PTB ABSOLUTE
L238A	6	76.87	84.27	.22	-.18	.95 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L360	6	76.92	84.47	.38	-.06	1.82 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L161	6	77.02	84.37	.39	.21	.94 65E DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, MGG (ZEISS) BASE
L255	#	78.16	86.04	2.34	.36	1.19 65D DIFFUSE REFLECTANCE, ELREPHO, NO TRAP, NRC-PTB ABSOLUTE

GMEANS: 76.58 84.28  
 95% ELLIPSE: 1.44 .62 WITH GAMMA = 39 DEGREES

BLUE REFLECTANCE, DIFFUSE, NO TRAP

SAMPLE J37 = 76.6 PERCENT

SAMPLE J35 = 84.3 PERCENT

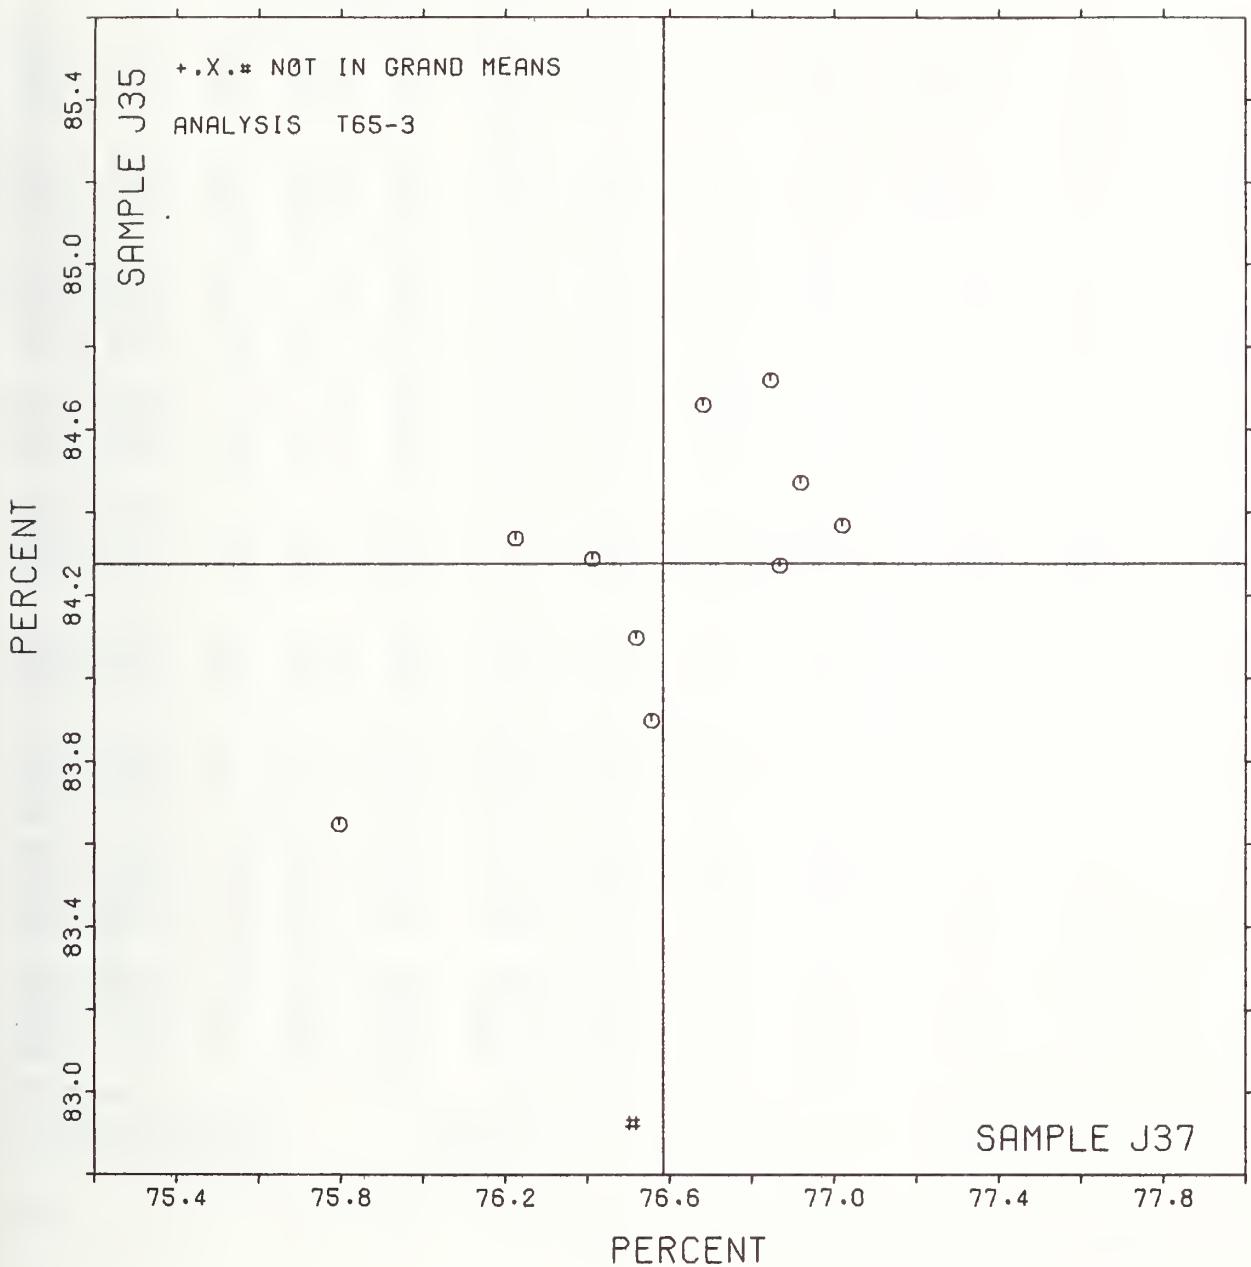

## ANALYSIS T75-1 TABLE 1

SPECULAR GLOSS AT 75 DEGREES, IN GLOSS UNITS

TAPPI STANDARD T480 GS-78, SPECULAR GLOSS OF PAPER AND PAPERBOARD AT 75 DEGREES

LAB CODE	SAMPLE E58	CAST COATED				SAMPLE J20	PRINTING				TEST D. = 10		
		211 GRAMS PER SQUARE METER	N. DEV	SDR	R. SDR		149 GRAMS PER SQUARE METER	N. DEV	SDR	R. SDR	VAR	F	LAB
L108	85.31	.99	.93	.27	.56	48.53	.85	.44	1.20	.87	75H	G	L108
L121	83.21	-1.11	-1.04	.27	.57	46.71	-.97	-.50	.97	.70	75H	G	L121
L122	83.24	-1.08	-1.01	.40	.83	46.50	-1.18	-.61	1.99	1.43	75H	G	L122
L128	84.00	-.32	-.30	.47	.98	48.70	1.02	.53	1.25	.90	75G	G	L128
L136	84.10	-.22	-.21	.23	.47	50.16	2.48	1.29	.93	.67	75G	G	L136
L153	84.40	.08	.07	.77	1.61	50.20	2.52	1.31	1.16	.84	75G	G	L153
L162	86.39	2.07	1.93	.26	.54	52.19	4.51	2.34	1.20	.87	75G	G	L162
L166	88.40	4.08	3.81	1.35	2.81	51.50	3.82	1.98	1.08	.78	75B	X	L166
L173A	86.10	1.78	1.66	.32	.66	46.90	-.78	-.41	1.60	1.15	75G	G	L173A
L182	84.67	.35	.33	.49	1.02	45.84	-1.84	-.96	1.86	1.34	75H	G	L182
L189	86.10	1.78	1.66	.74	1.54	50.50	2.82	1.46	.94	.68	75P	G	L189
L190R	83.43	-.89	-.83	.39	.80	47.82	.14	.07	1.21	.87	75G	G	L190R
L206	84.14	-.18	-.17	.29	.61	47.37	-.31	-.16	1.82	1.31	75H	G	L206
L210	85.81	1.49	1.39	.40	.84	48.69	1.01	.52	1.94	1.40	75H	G	L210
L211	83.48	-.84	-.78	.27	.55	48.43	.75	.39	1.60	1.16	75H	G	L211
L213	63.88	-.44	-.41	.29	.61	47.20	-.48	-.25	1.83	1.32	75H	G	L213
L223	84.94	.62	.58	.31	.64	47.18	-.50	-.26	1.29	.93	75B	G	L223
L224	82.92	-1.40	-1.31	.32	.66	43.50	-4.18	-2.17	1.58	1.14	75H	G	L224
L230	84.90	.58	.54	.32	.66	47.10	-.58	-.30	1.85	1.34	75H	G	L230
L243	84.30	-.02	-.02	.48	1.01	47.00	-.68	-.35	1.49	1.07	75B	G	L243
L251	83.15	-1.17	-1.09	.88	1.84	44.65	-3.03	-1.57	1.58	1.14	75G	G	L251
L253P	84.54	.22	.21	.30	.62	47.97	.29	.15	1.10	.80	75G	G	L253P
L255	84.60	.28	.26	.52	1.07	48.30	.62	.32	1.42	1.02	75H	G	L255
L256	84.08	-.24	-.22	.36	.76	47.40	-.28	-.15	1.83	1.32	75H	G	L256
L259	83.54	-.78	-.73	.34	.71	47.53	-.15	-.08	1.37	.99	75H	G	L259
L262	85.20	.88	.82	.42	.88	50.50	2.82	1.46	.97	.70	75K	G	L262
L278	84.41	.09	.08	.24	.50	49.88	2.20	1.14	1.57	1.13	75G	G	L278
L279	83.10	-1.22	-1.14	.32	.66	46.30	-1.38	-.72	1.16	.84	75G	G	L279
L291	83.27	-1.05	-.98	.21	.44	44.33	-3.35	-1.74	1.24	.89	75B	G	L291
L301	83.83	-.49	-.46	.44	.91	47.03	-.65	-.34	1.39	1.00	75H	G	L301
L315	85.00	.68	.64	.94	1.96	45.40	-2.28	-1.18	1.43	1.03	75G	G	L315
L317	86.25	1.93	1.80	.50	1.04	46.26	-1.42	-.74	1.14	.83	75H	G	L317
L321	96.65	12.33	11.52	3.24	6.75	54.10	6.42	3.33	.84	.61	75G	#	L321
L323	83.71	-.61	-.57	.40	.84	46.64	-1.04	-.54	1.16	.84	75H	G	L323
L328	88.43	4.11	3.84	.36	.75	47.46	-.22	-.12	1.96	1.41	75H	X	L328
L339	86.30	1.98	1.85	2.00	4.17	50.65	2.97	1.54	1.00	.72	75P	G	L339
L349	85.84	1.52	1.42	.58	1.20	48.52	.64	.33	1.57	1.13	75H	G	L349
L388	82.90	-1.42	-1.33	1.31	2.72	50.05	2.37	1.23	1.61	1.16	75P	G	L388
L396	83.40	-.92	-.86	.52	1.07	48.80	1.12	.58	1.48	1.06	75G	G	L396
L456	83.93	-.39	-.36	.22	.45	46.89	-.79	-.41	1.43	1.03	75H	G	L456
L483	79.33	-4.99	-4.66	1.83	3.82	45.23	-2.45	-1.27	1.87	1.35	75H	X	L483
L574	81.90	-2.42	-2.26	.57	1.18	45.50	-2.18	-1.13	.85	.61	75G	G	L574
L583	84.44	.12	.11	.36	.76	47.02	-.66	-.34	.64	.46	75H	G	L583
L587	84.80	.48	.45	.63	1.32	50.70	3.02	1.57	1.49	1.08	75H	G	L587
L592	83.73	-.59	-.55	.33	.69	45.08	-2.60	-1.35	1.35	.98	75H	G	L592
L643	84.19	-.13	-.12	.50	1.04	46.92	-.76	-.40	1.74	1.26	75H	G	L643
GR. MEAN = 84.32 GLOSS UNITS						GRAND MEAN = 47.68 GLOSS UNITS					TEST DETERMINATIONS = 10		
SD MEANS = 1.07 GLOSS UNITS						SD OF MEANS = 1.93 GLOSS UNITS					42 LABS IN GRAND MEANS		
AVERAGE SDR = .48 GLOSS UNITS						AVERAGE SDR = 1.39 GLOSS UNITS							
L250	87.70	3.38	3.16	.95	1.97	47.70	.02	.01	.67	.49	75Q	*	L250
L288	83.13	-1.19	-1.11	.07	.14	47.29	-.39	-.20	1.36	.98	75I	*	L288
TOTAL NUMBER OF LABORATORIES REPORTING = 48													

Best values: E58 84 ± 1 gloss units  
J20 47 ± 3 gloss units

The following laboratories were omitted from the grand means because of extreme test results: 321


ANALYSIS T75-1 TABLE 2  
SPECULAR GLOSS AT 75 DEGREES, IN GLOSS UNITS  
TAPPI STANDARD T480 6S-78, SPECULAR GLOSS OF PAPER AND PAPERBOARD AT 75 DEGREES

LAB CDDB	P	MEANS E58	COORDINATES J20	MAJOR MINOR	R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L483	X	79.33	45.23	-3.93	3.93	2.58 75H SPECULAR GLASS (75 DEGREE), HUNTER
L574	G	81.90	45.50	-2.65	1.58	.90 75G SPECULAR GLASS (75 DEGREE), GARDNER
L388	G	82.90	50.05	1.78	2.11	1.94 75P SPECULAR GLASS (75 DEGREE), PHOTOVOLT
L224	G	82.92	43.50	-4.41	-.03	.90 75H SPECULAR GLASS (75 DEGREE), HUNTER
L279	G	83.10	46.30	-1.70	.71	.75 75G SPECULAR GLASS (75 DEGREE), GARDNER
L288	*	83.13	47.29	-.76	1.00	.56 75I SPECULAR GLASS (75 DEGREE), HUNTER, 20 C, 65% RH
L251	G	83.15	44.65	-3.25	.13	1.49 75G SPECULAR GLASS (75 DEGREE), GARDNER
L121	G	83.21	46.71	-1.28	.74	.63 75H SPECULAR GLASS (75 DEGREE), HUNTER
L122	G	83.24	46.50	-1.47	.64	1.13 75H SPECULAR GLASS (75 DEGREE), HUNTER
L291	G	83.27	44.33	-3.51	-.09	.67 75H SPECULAR GLASS (75 DEGREE), HUNTER
L396	G	83.40	48.80	.76	1.23	1.07 75G SPECULAR GLASS (75 DEGREE), GARDNER
L190R	G	83.43	47.82	-.16	.89	.84 75G SPECULAR GLASS (75 DEGREE), GARDNER
L211	G	83.48	48.43	.44	1.04	.85 75H SPECULAR GLASS (75 DEGREE), HUNTER
L259	G	83.54	47.55	-.40	.69	.85 75H SPECULAR GLASS (75 DEGREE), HUNTER
L323	G	83.71	46.64	-1.18	.24	.84 75H SPECULAR GLASS (75 DEGREE), HUNTER
L592	G	83.73	45.08	-2.65	-.28	.84 75H SPECULAR GLASS (75 DEGREE), HUNTER
L301	G	83.83	47.03	-.78	.25	.96 75H SPECULAR GLASS (75 DEGREE), HUNTER
L213	G	83.88	47.20	-.60	.26	.96 75H SPECULAR GLASS (75 DEGREE), HUNTER
L456	G	83.93	46.89	-.88	.11	.74 75H SPECULAR GLASS (75 DEGREE), HUNTER
L128	G	84.00	48.70	.86	.63	.94 75G SPECULAR GLASS (75 DEGREE), GARDNER
L256	G	84.08	47.40	-.34	.14	1.04 75H SPECULAR GLASS (75 DEGREE), HUNTER
L136	G	84.10	50.16	2.27	1.01	.57 75G SPECULAR GLASS (75 DEGREE), GARDNER
L206	G	84.14	47.37	-.35	.07	.96 75H SPECULAR GLASS (75 DEGREE), HUNTER
L643	G	84.19	46.92	-.76	-.12	1.15 75H SPECULAR GLASS (75 DEGREE), HUNTER
L243	G	84.30	47.00	-.65	-.20	1.04 75B SPECULAR GLASS (75 DEGREE), BAUSCH + LOWE
L153	G	84.40	50.20	2.41	.74	1.22 75G SPECULAR GLASS (75 DEGREE), GARDNER
L278	G	84.41	49.88	2.11	.62	.82 75G SPECULAR GLASS (75 DEGREE), GARDNER
L583	G	84.44	47.02	-.59	-.33	.61 75H SPECULAR GLASS (75 DEGREE), HUNTER
L253P	G	84.54	47.97	.34	-.12	.71 75G SPECULAR GLASS (75 DEGREE), GARDNER
L255	G	84.60	48.30	.68	-.07	1.05 75H SPECULAR GLASS (75 DEGREE), HUNTER
L182	G	84.67	45.84	-1.63	-.93	1.18 75H SPECULAR GLASS (75 DEGREE), HUNTER
L587	G	84.80	50.70	3.01	.52	1.20 75H SPECULAR GLASS (75 DEGREE), HUNTER
L230	G	84.90	47.10	-.36	.74	1.00 75H SPECULAR GLASS (75 DEGREE), HUNTER
L223	G	84.94	47.18	-.27	.75	.78 75H SPECULAR GLASS (75 DEGREE), HUNTER
L315	G	85.00	45.40	-1.94	-1.38	1.50 75G SPECULAR GLASS (75 DEGREE), GARDNER
L262	G	85.20	50.50	2.95	.08	.79 75K SPECULAR GLASS (75 DEGREE), GAERTNER (K-C TYPE)
L108	G	85.31	48.53	1.12	-.66	.71 75H SPECULAR GLASS (75 DEGREE), HUNTER
L210	G	85.81	48.69	1.44	-.08	1.12 75H SPECULAR GLASS (75 DEGREE), HUNTER
L349	G	85.84	48.32	1.10	-1.23	1.17 75H SPECULAR GLASS (75 DEGREE), HUNTER
L173A	G	86.10	46.90	-.16	-1.94	.90 75G SPECULAR GLASS (75 DEGREE), GARDNER
L189	G	86.10	50.50	3.24	-.77	1.11 75P SPECULAR GLASS (75 DEGREE), PHOTOVOLT
L317	G	86.25	46.26	-.72	-2.29	.93 75H SPECULAR GLASS (75 DEGREE), HUNTER
L339	G	86.30	50.65	3.45	-.91	2.45 75P SPECULAR GLASS (75 DEGREE), PHOTOVOLT
L162	G	86.39	52.19	4.94	-.50	.70 75G SPECULAR GLASS (75 DEGREE), GARDNER
L250	*	87.70	47.70	1.11	-3.19	1.23 75Q SPECULAR GLASS (75 DEGREE), PHOTOVOLT, 20 C, 65% RH
L166	X	88.40	51.50	4.93	-2.63	1.79 75B SPECULAR GLASS (75 DEGREE), BAUSCH + LOWE
L328	X	88.43	47.46	1.12	-3.96	1.08 75H SPECULAR GLASS (75 DEGREE), HUNTER
L321	#	96.65	54.10	10.06	-9.60	3.68 75G SPECULAR GLASS (75 DEGREE), GARDNER

GMEANS: 84.32 47.68  
 95% ELLIPSE: 5.18 2.31 WITH GAMMA = 71 DEGREES

SPECULAR GLOSS, 75 DEGREE

SAMPLE E58 = 84.3 GLOSS UNITS      SAMPLE J20 = 47.7 GLOSS UNITS

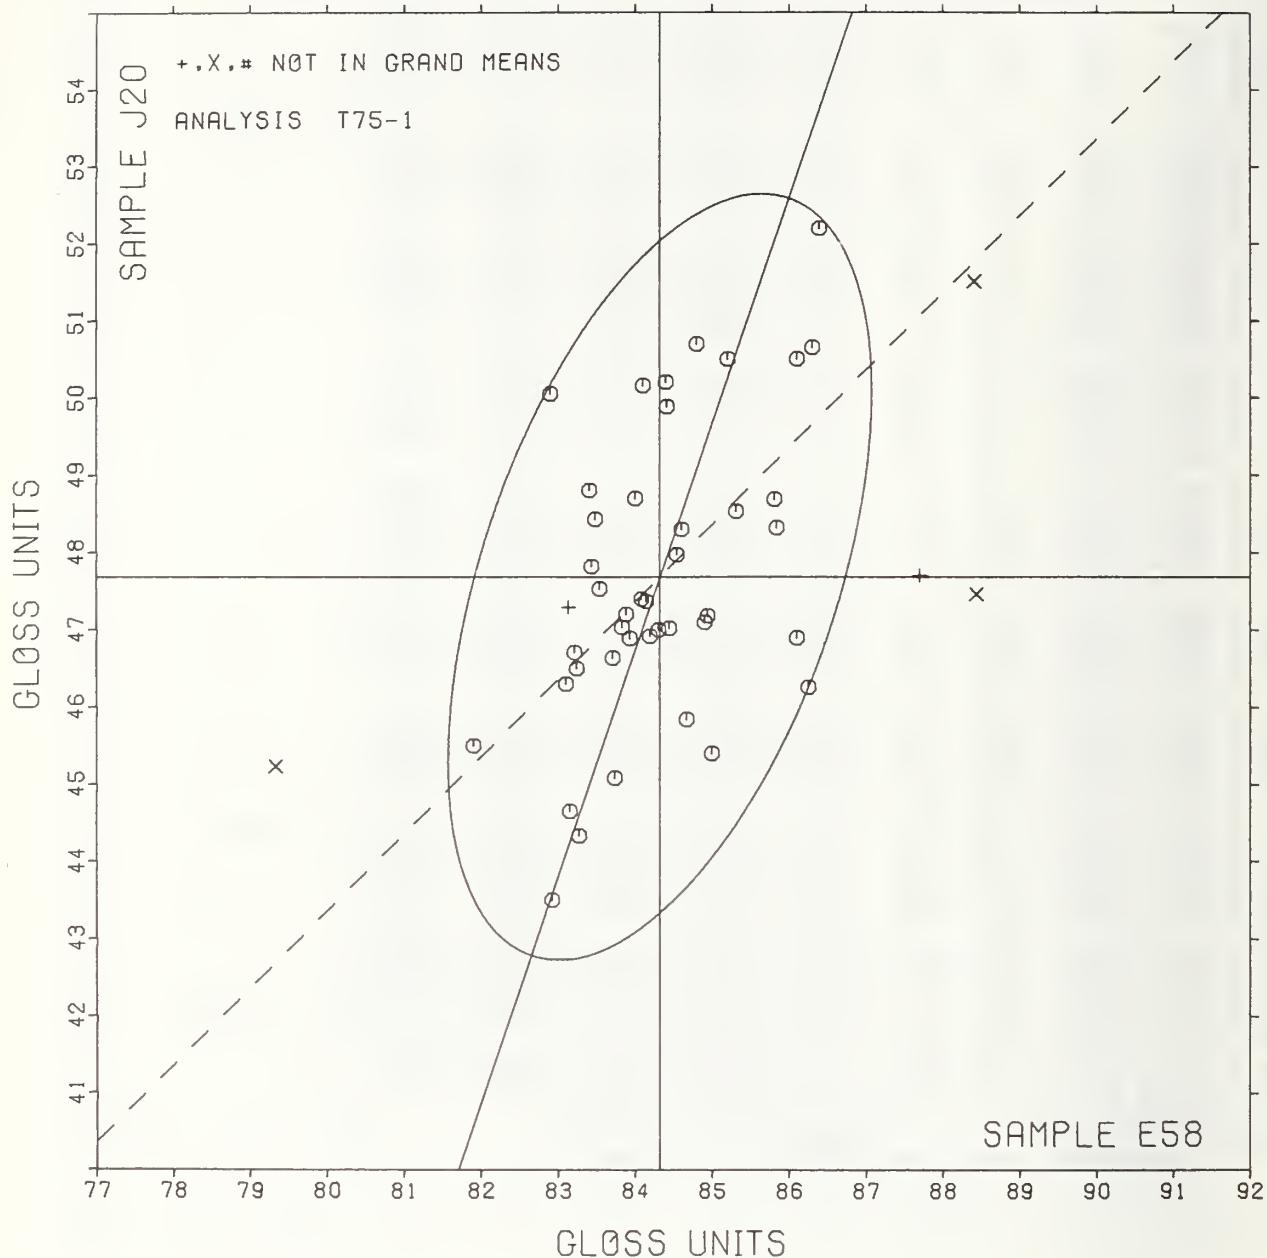

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T90-1 TABLE 1  
THICKNESS (CALIPER), THOUSANDS OF AN INCH  
TAPPI STANDARD T411 GS-76

JUNE 1978

LAB CGDE	SAMPLE J63	PRINTING				SAMPLE B28	BAG				TEST D. = 10		
		MEAN	DEV	N. DEV	SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F
L105	5.283	.005	.06	.038	.73	5.503	-.003	-.03	.113	1.12	90Q	Ø	L105
L118	5.292	.014	.17	.037	.71	5.623	.117	1.03	.059	.59	90V	Ø	L118
L122	5.235	-.043	-.50	.035	.68	5.565	.059	.52	.194	1.92	90V	Ø	L122
L123F	5.445	.167	1.96	.055	1.06	5.610	.104	.91	.122	1.21	90F	Ø	L123F
L125	5.302	.024	.28	.036	.70	5.618	.112	.98	.072	.71	90T	Ø	L125
L128	5.220	-.058	-.68	.023	.45	5.430	-.076	-.67	.088	.87	90T	Ø	L128
L131	5.410	.132	1.55	.032	.61	5.690	.184	1.62	.088	.87	90T	Ø	L131
L139	5.320	.042	.50	.048	.93	5.530	.024	.21	.134	1.32	90T	Ø	L139
L141	5.108	-.170	-2.00	.336	6.48	5.344	-.162	-.143	.095	.94	90T	Ø	L141
L153	5.353	.075	.88	.051	.99	5.447	-.059	-.52	.101	1.00	90T	Ø	L153
L158	5.330	.052	.61	.035	.67	5.640	.134	1.18	.077	.77	90T	Ø	L158
L159	5.309	.031	.37	.047	.91	5.491	-.015	-.14	.079	.78	90T	Ø	L159
L162	5.258	-.020	-.23	.041	.79	5.509	.003	.02	.068	.67	90D	Ø	L162
L166	5.288	.010	.12	.030	.57	5.529	.023	.20	.119	1.18	90T	Ø	L166
L173B	5.410	.132	1.55	.032	.61	5.630	.124	1.09	.116	1.15	90F	Ø	L173B
L174	5.320	.042	.50	.063	1.22	5.520	.014	.12	.140	1.38	90T	Ø	L174
L182	5.232	-.046	-.53	.055	1.06	5.378	-.128	-.13	.104	1.03	90L	Ø	L182
L190C	5.240	-.038	-.44	.052	1.00	5.420	-.086	-.76	.103	1.02	90T	Ø	L190C
L203A	5.250	-.028	-.33	.071	1.36	5.700	.194	1.71	.189	1.86	90T	*	L203A
L203C	5.340	.062	.73	.052	1.00	5.540	.034	.30	.117	1.16	90T	Ø	L203C
L213	5.330	.052	.61	.048	.93	5.570	.064	.56	.082	.81	90T	Ø	L213
L223	5.354	.076	.89	.035	.68	5.684	.178	1.57	.078	.77	90V	Ø	L223
L228	5.330	.052	.61	.048	.93	5.500	-.006	-.06	.163	1.61	90T	Ø	L228
L233	5.300	.022	.26	.044	.85	5.401	-.105	-.93	.109	1.08	90Q	Ø	L233
L238A	5.284	.006	.07	.044	.85	5.570	.064	.56	.078	.78	90T	Ø	L238A
L241	5.165	-.113	-1.33	.058	1.12	5.400	-.106	-.94	.158	1.56	90T	Ø	L241
L249	5.300	.022	.26	.050	.96	5.499	-.007	-.07	.101	1.00	90T	Ø	L249
L259	5.324	.046	.54	.041	.78	5.525	.019	.16	.129	1.27	90T	Ø	L259
L260	5.279	.001	.01	.022	.42	5.503	-.003	-.03	.100	.99	90T	Ø	L260
L261	5.395	.117	1.38	.064	1.24	5.570	.064	.56	.106	1.05	90T	Ø	L261
L262	5.265	-.013	-.15	.053	1.02	5.540	.034	.30	.070	.69	90T	Ø	L262
L285	5.170	-.108	-1.27	.067	1.30	5.380	-.126	-.12	.123	1.22	90T	Ø	L285
L291	5.395	.117	1.38	.044	.84	5.665	.159	1.40	.075	.74	90T	Ø	L291
L297	5.270	-.008	-.09	.026	.50	5.585	.079	.69	.106	1.04	90T	Ø	L297
L305	5.175	-.103	-1.21	.082	1.59	5.180	-.326	-.288	.193	1.91	90T	*	L305
L309	5.240	-.038	-.44	.052	1.00	5.440	-.066	-.59	.117	1.16	90T	Ø	L309
L318	5.210	-.068	-.80	.066	1.27	5.495	-.011	-.10	.172	1.70	90T	Ø	L318
L323	5.187	-.091	-1.07	.043	.82	5.474	-.032	-.29	.058	.58	90T	Ø	L323
L324	5.300	.022	.26	.053	1.02	5.520	.014	.12	.116	1.15	90T	Ø	L324
L326	5.425	.147	1.73	.049	.94	5.545	.039	.34	.086	.85	90T	Ø	L326
L328	5.280	.002	.03	.063	1.22	5.530	.024	.21	.116	1.15	90T	Ø	L328
L331	5.303	.025	.30	.046	.88	5.463	-.043	-.38	.137	1.35	90T	Ø	L331
L339	5.200	-.078	-.91	.047	.91	5.580	.074	.65	.079	.78	90T	Ø	L339
L341	5.378	.100	1.18	.024	.46	5.696	.190	1.67	.108	1.07	90T	Ø	L341
L352	5.332	.054	.64	.030	.58	5.602	.096	.84	.147	1.45	90Q	Ø	L352
L356	5.163	-.115	-1.35	.029	.55	5.418	-.088	-.78	.077	.77	90T	Ø	L356
L358	5.273	-.005	-.06	.059	1.13	5.497	-.009	-.08	.074	.73	90T	Ø	L358
L372	5.280	.002	.03	.042	.81	5.450	-.056	-.50	.071	.70	90T	Ø	L372
L376	5.220	-.058	-.68	.042	.81	5.480	-.026	-.23	.079	.78	90T	Ø	L376
L380	5.260	-.018	-.21	.039	.76	5.520	.014	.12	.103	1.02	90T	Ø	L380
L382	5.390	.112	1.32	.032	.61	5.640	.134	1.18	.097	.96	90T	Ø	L382
L390	5.170	-.108	-1.27	.116	2.24	5.280	-.226	-.200	.092	.91	90T	Ø	L390
L556	5.060	-.218	-2.56	.024	.46	5.254	-.252	-.23	.103	1.02	90T	*	L556
L557	5.265	-.013	-.15	.063	1.21	5.365	-.141	-.125	.118	1.17	90T	Ø	L557
L558	5.330	.052	.61	.048	.93	5.750	.244	2.15	.097	.96	90T	*	L558
L559	5.318	.040	.47	.042	.81	5.535	.029	.25	.068	.67	90T	Ø	L559
L560	5.300	.022	.26	.067	1.29	5.450	-.056	-.50	.071	.70	90T	Ø	L560
L561	5.260	-.018	-.21	.084	1.63	5.450	-.056	-.50	.127	1.25	90T	Ø	L561
L567	5.376	.098	1.15	.048	.92	5.563	.057	.50	.053	.52	90V	Ø	L567
L574	5.154	-.124	-1.45	.049	.95	5.432	-.074	-.66	.105	1.04	90V	Ø	L574
L575	5.199	-.079	-.93	.047	.92	5.367	-.139	-.23	.086	.85	90T	Ø	L575
L581	5.365	.087	1.02	.034	.65	5.600	.094	.83	.058	.57	90T	Ø	L581
L587	5.250	-.028	-.33	.053	1.02	5.440	-.066	-.59	.084	.83	90T	Ø	L587
L626	5.012	-.266	-3.12	.048	.93	5.288	-.218	-.93	.090	.89	90T	*	L626

GR. MEAN = 5.278 MILS

SD MEANS = .085 MILS

AVERAGE SDR = .052 MILS

GR. MEAN = 134.06 MICRÖMETER

GRAND MEAN = 5.506 MILS

SD OF MEANS = .113 MILS

AVERAGE SDR = .101 MILS

GRAND MEAN = 139.86 MICRÖMETER

TEST DETERMINATIONS = 10

64 LABS IN GRAND MEANS

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T90-1 TABLE 1  
THICKNESS (CALIPER), THOUSANDS OF AN INCH  
TAPPI STANDARD T411 GS-76

JUNE 1978

LAB CODE	SAMPLE J63	PRINTING					SAMPLE B28	BAG					TEST D. = 10		
		MEAN	DEV	N. DEV	SDR	R. SDR		MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L185	5.347	.069	.81	.078	1.51		5.332	-.174	-1.54	.048	.48	90B	♦	L185	
L203B	5.070	-.208	-2.44	.106	2.04		5.200	-.306	-2.70	.211	2.08	90C	♦	L203B	
L243	5.325	.047	.55	.049	.94		5.495	-.011	-.10	.130	1.29	90S	♦	L243	
L251	5.193	-.085	-1.00	.031	.60		5.358	-.148	-1.31	.053	.52	90W	♦	L251	
L322	5.170	-.108	-1.27	.149	2.88		5.550	-.044	.38	.242	2.39	90U	♦	L322	
L330	5.380	.102	1.20	.132	2.54		5.770	.264	2.33	.206	2.03	90U	♦	L330	
L344	5.390	.112	1.32	.057	1.10		5.640	.134	1.18	.151	1.49	90U	♦	L344	
L396M	5.090	-.188	-2.21	.057	1.10		4.800	-.706	-6.23	.105	1.04	90S	♦	L396M	
L484	5.283	.006	.07	.045	.86		5.394	-.113	-1.00	.072	.71	90B	♦	L484	
L562	5.295	.017	.20	.069	1.32		5.410	-.096	.85	.081	.80	90C	♦	L562	
TOTAL NUMBER OF LABORATORIES REPORTING = 76															

Best values: J63 5.28 ± 0.13 mils  
B28 5.50 ± 0.19 mils

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T90-1 TABLE 2  
THICKNESS (CALIPER), THOUSANDTHS OF AN INCH  
TAPPI STANDARD T411 GS=76

JUNE 1978

LAB CGDE	P	MEANS J63	MEANS B28	COORDINATES	AVG	R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
MAJOR	MINOR						
L616	*	5.000	5.130	-.468	.018	.81	90C THICKNESS (CALIPER), CADY, HAND DRIVEN
L626	*	5.012	5.288	-.330	.097	.91	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L556	*	5.060	5.254	-.331	.038	.74	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L203B	*	5.070	5.200	-.370	-.000	2.06	90C THICKNESS (CALIPER), CADY, HAND DRIVEN
L396M	*	5.090	4.800	-.690	-.242	1.07	90S THICKNESS (CALIPER), SCHOPPER, HAND DRIVEN
L141	Ø	5.108	5.344	-.230	.049	3.71	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L574	Ø	5.154	5.432	-.131	.061	1.00	90V THICKNESS (CALIPER), TMI, MOTOR DRIVEN, DIGITIZED
L356	Ø	5.163	5.418	-.138	.045	.66	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L241	Ø	5.165	5.400	-.151	.033	1.34	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L322	*	5.170	5.550	-.025	.114	2.64	90U THICKNESS (CALIPER), TMI, HAND DRIVEN
L390	Ø	5.170	5.280	-.248	-.038	1.57	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L285	Ø	5.170	5.380	-.165	.018	1.26	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L305	*	5.175	5.180	-.328	-.098	1.75	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L323	Ø	5.187	5.474	-.078	.057	.70	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L251	*	5.193	5.358	-.170	-.013	.56	90W THICKNESS (CALIPER), L + W, MOTOR DRIVEN, 20 C, 65% RH
L575	Ø	5.199	5.367	-.160	-.013	.88	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L339	Ø	5.200	5.580	.017	.106	.84	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L318	Ø	5.210	5.495	-.048	.050	1.49	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L376	Ø	5.220	5.480	-.054	.033	.80	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L128	Ø	5.220	5.430	-.096	.005	.66	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L182	Ø	5.232	5.378	-.132	-.035	1.04	90L THICKNESS (CALIPER), L + W, MOTOR DRIVEN
L122	Ø	5.235	5.565	.024	.068	1.30	90V THICKNESS (CALIPER), TMI, MOTOR DRIVEN, DIGITIZED
L190C	Ø	5.240	5.420	-.093	-.017	1.01	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L309	Ø	5.240	5.440	-.076	-.006	1.08	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L576	*	5.249	4.878	-.536	-.329	.91	90C THICKNESS (CALIPER), CADY, HAND DRIVEN
L587	Ø	5.250	5.440	-.071	-.014	.93	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L203A	*	5.250	5.700	.144	.132	1.61	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L162	Ø	5.258	5.509	-.009	.018	.73	90D THICKNESS (CALIPER), CADY, MOTOR DRIVEN
L561	Ø	5.260	5.450	-.057	-.017	1.44	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L380	Ø	5.260	5.520	.001	.022	.89	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L557	Ø	5.265	5.365	-.124	-.069	1.19	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L262	Ø	5.265	5.540	.021	.029	.86	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L297	Ø	5.270	5.585	.061	.051	.77	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L358	Ø	5.273	5.497	-.011	-.001	.93	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L260	Ø	5.279	5.503	-.002	-.003	.71	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L372	Ø	5.280	5.450	-.045	-.034	.76	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L328	Ø	5.280	5.530	.021	.011	1.18	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L105	Ø	5.283	5.503	.000	-.006	.92	90Q THICKNESS (CALIPER), EMVECG, MOTOR DRIVEN
L484	*	5.283	5.394	-.090	-.068	.79	90E THICKNESS (CALIPER), SCHOPPER, HAND DRIVEN
L238A	Ø	5.284	5.570	.056	.031	.81	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L166	Ø	5.288	5.529	.024	.004	.88	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L118	Ø	5.292	5.623	.104	.054	.65	90V THICKNESS (CALIPER), TMI, MOTOR DRIVEN, DIGITIZED
L562	*	5.295	5.410	-.070	-.068	1.06	90C THICKNESS (CALIPER), CADY, HAND DRIVEN
L249	Ø	5.300	5.499	.006	-.023	.98	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L324	Ø	5.300	5.520	.024	-.011	1.08	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L560	Ø	5.300	5.450	-.034	-.050	.99	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L233	Ø	5.300	5.401	-.075	-.078	.96	90Q THICKNESS (CALIPER), EMVECG, MOTOR DRIVEN
L125	Ø	5.302	5.618	.106	.043	.71	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L331	Ø	5.303	5.463	-.022	-.045	1.12	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L159	Ø	5.309	5.491	.005	-.034	.84	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L559	Ø	5.318	5.535	.046	-.017	.74	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L174	Ø	5.320	5.520	.035	-.027	1.30	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L139	Ø	5.320	5.530	.043	-.022	1.13	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L259	Ø	5.324	5.525	.041	-.028	1.03	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L243	*	5.325	5.495	.017	-.045	1.11	90S THICKNESS (CALIPER), SCHOPPER, HAND DRIVEN
L228	Ø	5.330	5.500	.024	-.047	1.27	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L213	Ø	5.330	5.570	.082	-.007	.87	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L558	*	5.330	5.750	.231	.094	.95	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L158	Ø	5.330	5.640	.140	.032	.72	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L352	Ø	5.332	5.602	.109	.009	1.02	90Q THICKNESS (CALIPER), EMVECG, MOTOR DRIVEN
L203C	Ø	5.340	5.540	.063	-.033	1.08	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L185	*	5.347	5.332	-.105	-.155	.99	90B THICKNESS (CALIPER), ANTHOR, HAND DRIVEN
L153	Ø	5.353	5.447	-.007	-.096	.99	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN
L223	Ø	5.354	5.684	.190	.037	.72	90V THICKNESS (CALIPER), TMI, MOTOR DRIVEN, DIGITIZED
L581	Ø	5.365	5.600	.126	-.020	.61	90T THICKNESS (CALIPER), TMI, MOTOR DRIVEN

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T90-1 TABLE 2  
THICKNESS (CALIPER), THOUSANDS OF AN INCH  
TAPPI STANDARD T411 GS-76

JUNE 1978

LAB CODE	F	MEANS		COORDINATES			AVG	PROPERTY---TEST INSTRUMENT---CONDITIONS		
		J63	B28	MAJOR	MINOR	R.SDR	VAR			
L567	6	5.376	5.563	.102	-.049	.72	90V	THICKNESS (CALIPER), TMI,	MOTOR DRIVEN, DIGITIZED	
L341	6	5.378	5.696	.213	.024	.76	90T	THICKNESS (CALIPER), TMI,	MOTOR DRIVEN	
L330	+	5.380	5.770	.275	.064	2.29	90U	THICKNESS (CALIPER), TMI,	HAND DRIVEN	
L382	6	5.390	5.640	.174	-.018	.78	90T	THICKNESS (CALIPER), TMI,	MOTOR DRIVEN	
L344	+	5.390	5.640	.174	-.018	1.29	90U	THICKNESS (CALIPER), TMI,	HAND DRIVEN	
L261	6	5.395	5.570	.118	-.061	1.14	90T	THICKNESS (CALIPER), TMI,	MOTOR DRIVEN	
L291	6	5.395	5.665	.197	-.008	.79	90T	THICKNESS (CALIPER), TMI,	MOTOR DRIVEN	
L173B	6	5.410	5.630	.176	-.040	.88	90F	THICKNESS (CALIPER), FEDERAL,	MOTOR DRIVEN	
L131	6	5.410	5.690	.226	-.006	.74	90T	THICKNESS (CALIPER), TMI,	MOTOR DRIVEN	
L326	6	5.425	5.545	.115	-.100	.90	90T	THICKNESS (CALIPER), TMI,	MOTOR DRIVEN	
L123F	6	5.445	5.610	.180	-.080	1.13	90F	THICKNESS (CALIPER), FEDERAL,	MOTOR DRIVEN	
GMEANS:		5.278	5.506			1.00				
		95% ELLIPSE:		.336	.125		WITH GAMMA = 55 DEGREES			


THICKNESS (CALIPER)

SAMPLE J63 = 5.28 MILS

SAMPLE J63 = 134.1 MICRØMETER

SAMPLE B28 = 5.51 MILS

SAMPLE B28 = 139.9 MICRØMETER

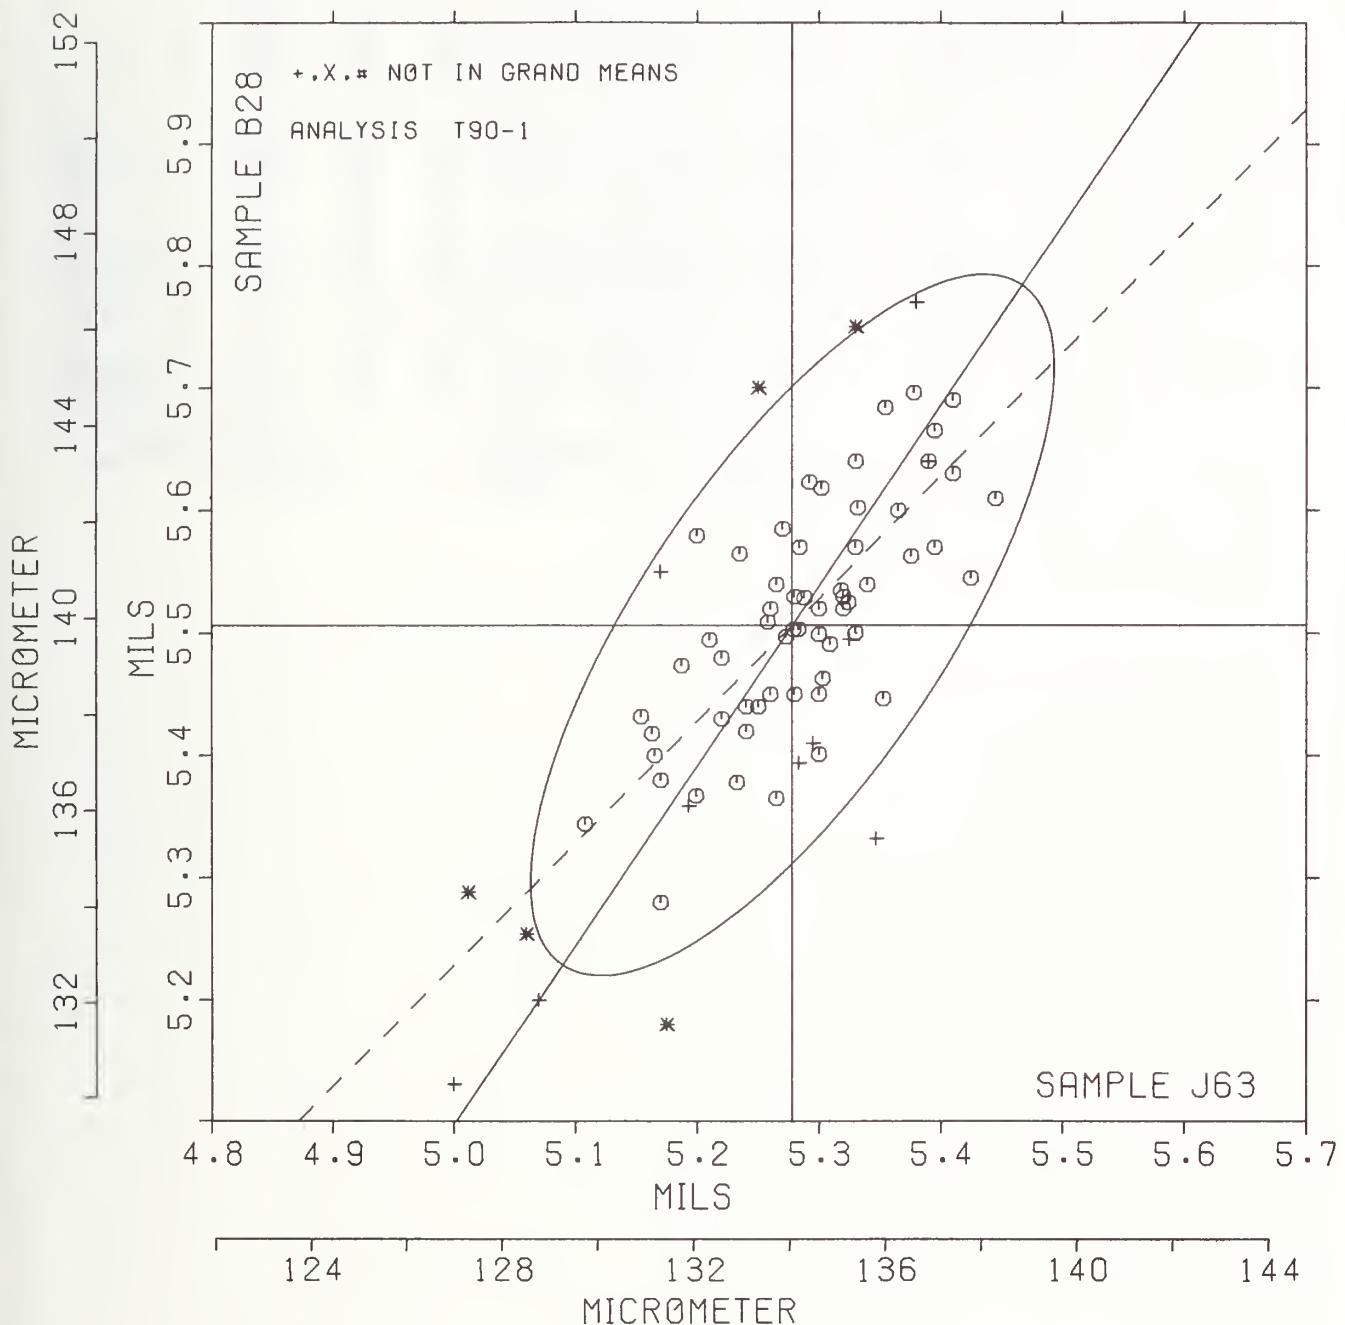

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T95-1 TABLE 1  
GRAMMAGE (MASS PER UNIT AREA)  
TAPPI STANDARD T410 GS-68

JUNE 1978

LAB CODE	SAMPLE KRAFT D28 96 GRAMS PER SQUARE METER					SAMPLE KRAFT D29 123 GRAMS PER SQUARE METER					TEST D.= 10		
	MEAN	DEV	N.DEV	SDR	R.SDR	MEAN	DEV	N.DEV	SDR	R.SDR	VAR	F	LAB
L121	96.13	.38	.57	.85	1.16	124.30	-.06	-.09	.54	.94	95B	6	L121
L162	6.25	-89.50	-132.56	.00	.00	8.25	-116.11	-191.06	.00	.00	95K	#	L162
L213	95.61	-.14	-.20	.68	.93	124.10	-.26	-.42	.80	1.40	95F	6	L213
L233	107.04	11.29	16.73	.35	.48	139.81	15.45	25.43	.58	1.01	95T	#	L233
L249	96.04	.29	.44	.55	.74	125.00	.64	1.06	.00	.00	95I	6	L249
L280	95.82	.07	.11	.55	.74	124.78	.42	.70	.87	1.51	95T	6	L280
L297	94.63	-1.11	-1.65	.29	.39	123.67	-.69	-1.14	.58	1.00	95C	6	L297
L305	96.79	1.04	1.55	.75	1.02	124.96	.60	.99	.63	1.10	95T	6	L305
L339	96.34	.59	.88	.30	.40	124.80	.44	.73	.00	.00	95T	6	L339
L344	96.04	.30	.44	.32	.43	125.03	.68	1.11	.29	.50	95T	6	L344
L557	96.30	.55	.81	1.11	1.52	96.23	-28.12	-46.28	.99	1.71	95A	#	L557
L558	94.92	-.83	-1.23	.79	1.07	123.59	-.77	-1.26	.94	1.64	95A	6	L558
L559	95.07	-.68	-1.00	.33	.45	123.23	-1.13	-1.85	.61	1.05	95D	6	L559
L560	93.27	-2.48	-3.67	.82	1.12	120.94	-3.42	-5.62	.41	.72	95A	#	L560
L561	95.78	.03	.05	1.57	2.14	125.00	.64	1.06	1.14	1.98	95T	6	L561
L597	96.60	.85	1.26	1.29	1.76	124.40	.04	.07	.00	.00	95C	6	L597
L616	95.92	.18	.26	.82	1.11	124.38	.02	.04	.83	1.44	95T	6	L616
L625	94.75	-1.00	-1.48	1.21	1.64	123.75	-.61	-1.00	.83	1.44	95E	6	L626
GR. MEAN = 95.75 G/SQ.METER					GRAND MEAN = 124.36 G/SQ.METER					TEST DETERMINATIONS = 10			
SD MEANS = .68 G/SQ.METER					SD OF MEANS = .61 G/SQ.METER					14 LABS IN GRAND MEANS			
AVERAGE SDR = .73 G/SQ.METER					AVERAGE SDR = .58 G/SQ.METER								
TOTAL NUMBER OF LABORATORIES REPORTING = 18													

Best values: D28 95.9 + 1.2 grams per square meter  
D29 124.4 + 0.9 grams per square meter

The following laboratories were omitted from the grand means because of extreme test results: 233, 557, 560

Data from the following laboratories appear to be off by a multiplicative factor: 162

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS T95-1 TABLE 2  
 GRAMMAGE (MASS PER UNIT AREA)  
 TAPPI STANDARD T410 GS-68


JUNE 1978

LAB CODE	F	MEANS D28	MEANS D29	COORDINATES MAJOR	COORDINATES MINOR	AVG R.SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS
L162	#	6.25	8.25	-143.79	-28.53	.00	95K BASIS WEIGHT (GRAMMAGE), WEIGHED AS RECEIVED
L560	#	93.27	120.94	-4.11	-.94	.92	95A BASIS WEIGHT (GRAMMAGE), CHANDLER + PRICE PAPER CUTTER
L297	Ø	94.63	123.67	-1.29	.21	.70	95C BASIS WEIGHT (GRAMMAGE), CUTTING BOARD
L626	Ø	94.75	123.75	-1.15	.20	1.54	95B BASIS WEIGHT (GRAMMAGE), GUILLOTINE TYPE CUTTER
L558	Ø	94.92	123.59	-1.13	-.03	1.35	95A BASIS WEIGHT (GRAMMAGE), CHANDLER + PRICE PAPER CUTTER
L559	Ø	95.07	123.23	-1.25	-.40	.75	95D BASIS WEIGHT (GRAMMAGE), DIE CUT
L213	Ø	95.61	124.10	-.27	-.10	1.16	95F BASIS WEIGHT (GRAMMAGE), FIGUR-SQUARE CUTTER
L561	Ø	95.78	125.00	.45	.46	2.06	95T BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L280	Ø	95.82	124.78	.33	.27	1.13	95T BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L616	Ø	95.92	124.38	.15	-.10	1.27	95T BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L249	Ø	96.04	125.00	.64	.29	.37	95I BASIS WEIGHT (GRAMMAGE), INGENCO PAPER CUTTER
L344	Ø	96.04	125.03	.67	.31	.47	95T BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L121	Ø	96.13	124.30	.25	-.30	1.05	95B BASIS WEIGHT (GRAMMAGE), CONCOR CUTTER
L557	#	96.30	96.23	-18.09	-21.54	1.61	95A BASIS WEIGHT (GRAMMAGE), CHANDLER + PRICE PAPER CUTTER
L339	Ø	96.34	124.80	.74	-.06	.20	95T BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L597	Ø	96.60	124.40	.67	-.53	.88	95C BASIS WEIGHT (GRAMMAGE), CUTTING BOARD
L305	Ø	96.79	124.96	1.18	-.23	1.06	95T BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L233	#	107.04	139.81	18.67	4.20	.75	95T BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
GMEANS:		95.75	124.36		1.00		
95% ELLIPSE:		2.49		.87			WITH GAMMA = 41 DEGREES

## GRAMMAGE (MASS PER UNIT AREA)

SAMPLE 028 = 95.7 G/SQ.METER

SAMPLE D29 = 124.4 G/SQ.METER

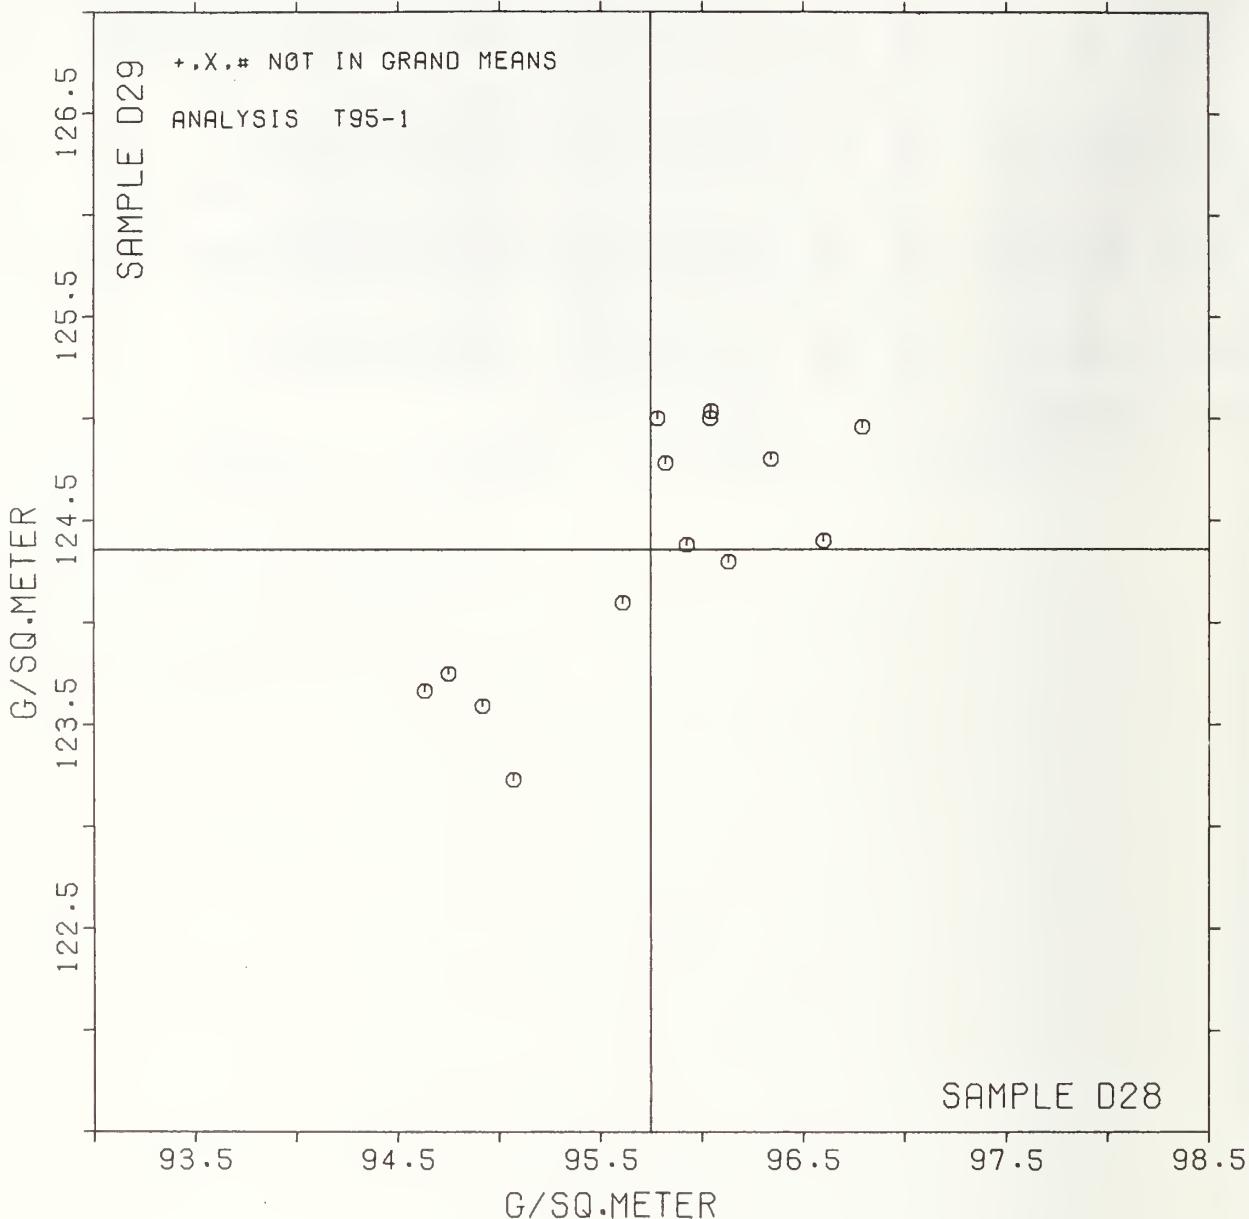

## SUMMARY TABLE

TEST METHOD		SAMPLE CODE	GRAND MEAN	SD GP MEAN	AVER SDR	REPL CRP	LABS INCL	LABS PARTIC	REPL TAPPI	REPEAT	REPROD
AIR RESISTANCE, GURLEY T40-1	GURLEY UNITS	J47 E73	30.0 17.5	1.1 1.1	1.5 1.5	10	50	55	10	1.3 1.3	2.9 3.1
AIR RESISTANCE, SHEFFIELD T40-2	SHEPP. UNITS	J47 E73	106.3 157.9	4.7 7.1	4.0 11.1	10	38	43	10	3.5 9.7	13.0 19.6
AIR RESISTANCE, GURLEY HG PLATATION T41-1	SEC/10 CC	B37 B73	755. 1078.	39. 248.	79. 415.	10	13	14	10	69. 363.	107. 687.
SMOOTHNESS, PARKER PRINTSURF T44-1	MICRONS	H45 J12	5.95 5.05	.46 .28	.10 .23	10	7	7	10	.09 .20	1.27 .79
SMOOTHNESS, SHEFFIELD T45-1	SHEPP. UNITS	H45 J12	262.9 143.0	9.8 6.7	9.1 11.1	15	78	86	10	7.9 9.7	27.5 19.3
SMOOTHNESS, BEKK T45-2	BEKK SECONDS	H45 J12	15.20 32.78	1.26 2.25	.80 4.35	15	7	13	10	.70 3.81	3.52 6.62
SMOOTHNESS, BENDTSEN T47-1	ML/MIN	H45 J12	460. 176.	120. 15.	42. 24.	10	9	9	10	37. 21.	332. 41.
K & N INK ABSORPTION T56-1	K & N UNITS	B80 E50	23.20 64.09	3.05 4.61	.66 .33	4	6	8	4	.92 .46	8.46 12.76
PH, COLD T57-1	PH UNITS	J77 J14	7.31 7.31	.35 .40	.09 .05	5	6	6	2	.18 .11	.99 1.11
PH, HOT T57-2	PH UNITS	J77 J14	7.748 7.756	.127 .066	.053 .067	5	4	6	2	.104 .131	.361 .210
OPACITY, B&L TYPE, 89% BACKING T60-1	PERCENT	E40 J57	96.16 92.74	.31 .54	.21 .37	10	74	67	5	.26 .46	.89 1.53
OPACITY, B&L TYPE, PAPER BACKING T60-2	PERCBNT	E40 J57	96.07 92.97	.15 .34	.24 .30	10	7	7	5	.30 .37	.47 .97
OPACITY, ELREPHO TYPE, PAPER BACKING T60-3	PERCENT	E40 J57	96.69 93.55	.10 .18	.10 .18	10	6	10	5	.12 .23	.29 .51
BLUE REFLECTANCE, DIRECTIONAL T65-1	PERCENT	J37 J35	75.79 83.98	.42 .44	.16 .14	8	20	42	6	.18 .16	1.17 1.23
BLUE REFLECTANCE, DIFFUSE, WITH TRAP T65-2	PERCENT	J37 J35	75.43 84.43	.29 .14	.15 .09	8	10	15	6	.17 .10	.82 .40
BLUE REFLECTANCE, DIFFUSE, NO TRAP T65-3	PERCENT	J37 J35	76.58 84.28	.37 .33	.11 .06	8	10	13	6	.13 .07	1.03 .91
SPECULAR GLOSS, 75 DEGREE T75-1	GLOSS UNITS	E58 J20	84.32 47.68	1.07 1.93	.48 1.39	10	42	48	5	.60 1.72	2.99 5.47
THICKNESS (CALIPER) T90-1	MILS	J63 B28	5.278 5.506	.085 .113	.052 .101	10	64	76	10	.045 .089	.236 .314
GRAMMAGE (MASS PER UNIT AREA) T95-1	G/SQ. METER	D28 D29	95.75 124.36	.68 .61	.73 .58	10	14	18	3	1.17 .92	2.11 1.85

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET		1. PUBLICATION OR REPORT NO.  TAPPI CRP 54G	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE  Technical Association of the Pulp and Paper Industry COLLABORATIVE REFERENCE PROGRAM FOR PAPER Report #54G		5. Publication Date September 22, 1978		
7. AUTHOR(S)  R. G. Powell, E. B. Randall, Jr., J. Horlick		6. Performing Organization Code  NBSIR 78-1350		
9. PERFORMING ORGANIZATION NAME AND ADDRESS  NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		8. Performing Organ. Report No.  10. Project/Task/Work Unit No. 7825578 11. Contract/Grant No.		
12. Sponsoring Organization Name and Complete Address (Street, City, State, ZIP)  Collaborative Testing Services, Inc., 9241 Wood Glade Drive, Great Falls, Virginia 22066; and Technical Association of the Pulp and Paper Industry		13. Type of Report & Period Covered Final 14. Sponsoring Agency Code		
15. SUPPLEMENTARY NOTES				
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.)  Collaborative Reference Programs provide participating laboratories with the means for checking periodically the level and uniformity of their testing in comparison with that of other participating laboratories. An important by-product of the programs is the provision of realistic pictures of the state of the testing art. This is one of the periodic reports showing averages for each participant, within and between laboratory variability, and other information for participants and standards committees.				
17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons)  Collaborative reference program; Laboratory evaluation; Paper; Precision; Reference samples, Testing calibration				
18. AVAILABILITY  <input type="checkbox"/> Unlimited  <input checked="" type="checkbox"/> For Official Distribution. Do Not Release to NTIS  <input type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office Washington, D.C. 20402, SD Stock No. SN003-003  <input type="checkbox"/> Order From National Technical Information Service (NTIS) Springfield, Virginia 22151		19. SECURITY CLASS (THIS REPORT)  UNCL ASSIFIED		21. NO. OF PAGES  56
		20. SECURITY CLASS (THIS PAGE)  UNCLASSIFIED		22. Price