


NBS 12-79-1358



TECHNICAL ASSOCIATION OF THE
PULP AND PAPER INDUSTRY

COLLABORATIVE REFERENCE PROGRAM
FOR PAPER

REPORT NO. 55S
STRENGTH TESTS



U.S. DEPARTMENT OF COMMERCE
National Bureau of Standards

NBS COLLABORATIVE REFERENCE PROGRAMS

TAPPI Paper and Board (6 times per year)

Bursting strength	Smoothness
Tearing strength	Surface pick strength
Tensile breaking strength	K & N ink absorption
Elongation to break	pH
Tensile energy absorption	Opacity
Folding endurance	Blue reflectance (brightness)
Stiffness	Specular gloss, 75°
Air resistance	Thickness
Grammage	Concora (flat crush)
	Ring crush

FKBG-API Containerboard (48 times per year)

Mullen burst of linerboard
Concora test of medium

MCCA Color and Appearance (4 times per year)

Gloss at 60°
Color and color difference
Retroreflectivity

Rubber (4 times per year)

Tensile strength, ultimate elongation and tensile stress
Hardness
Mooney viscosity
Vulcanization properties

ASTM Textiles (3 times per year)

Flammability (FF3-71 and FF5-74)

ASTM Cement (2 times per year)

Chemical (11 chemical components)
Physical (8 characteristics)

AASHTO Bituminous

Asphalt cement (2 times per year)
Cutbacks (once a year)



Collaborative Reference Programs
B360 Polymer Building
National Bureau of Standards
Washington, D.C. 20234

TECHNICAL ASSOCIATION OF THE
PULP AND PAPER INDUSTRY

**COLLABORATIVE REFERENCE PROGRAM
FOR PAPER**

Report No. 55S
STRENGTH TESTS

R. G. Powell
TAPPI-NBS Research Associate
Collaborative Testing Services, Inc.

J. Horlick
Office of Testing Laboratory Evaluation Technology
Office of Engineering Standards
National Engineering Laboratory

NBSIR 79-1358

U. S. DEPARTMENT OF COMMERCE
National Bureau of Standards

TAPPI-NBS COLLABORATIVE REFERENCE PROGRAM

BACKGROUND AND PURPOSE

In 1969, the National Bureau of Standards and the Technical Association of the Pulp and Paper Industry established a collaborative reference program to provide a participating laboratory with a means to check periodically the level and uniformity of its testing in comparison with that of other laboratories.

The interchange of paper and board products and of the raw materials for these products requires agreement among raw material suppliers, paper and board producers, converters, distributors, retailers, commercial testing laboratories, user organizations and the ultimate consumer as to the meaning of test results, an agreement that cannot be achieved without accurate and precise testing. This program is designed to help assure agreement.

HOW THE PROGRAM WORKS

Participants Select the Tests in which they wish to participate. This choice is made on joining the program, but additional tests may be added at any time. Also new participants may enter the program at any time.

Test Samples are Distributed Bimonthly; i.e. every 2 months.

Provisional Values are Provided with the Samples for one or both of the test levels, depending on method. The provisional values permit serious discrepancies to be detected without delay. (It is left to the discretion of the laboratory supervisor as to whether these values should be known to the operator.)

Each Participant Tests the Samples, following instructions provided for each test method. The full check on a single instrument should normally take no more than 30 minutes. The test results are then sent to NBS for analysis. The participant is also asked to report other information relevant to an accurate analysis, such as test conditions and the instruments used.

Industry Means, Best Values and Other Statistics are developed from the data by NBS. The best values are estimates based on a careful examination of all data, both current and past, with special attention to results obtained by the National Bureau of Standards and other recognized reference laboratories in this and other countries.

A Quick Report is Prepared for each participating laboratory reporting data on time. This report shows the industry mean values, and the deviations of the laboratory's results from these values for each test method.

A Longer Summary Report, Showing the Data from all Participants, is also prepared. In the summary report, of which this report is an example, each laboratory is identified by a code number so that the information is maintained on a confidential basis. However, instruments are identified by type so participants can compare their results with those obtained on similar instruments of different manufacture. This report includes test averages, best values and standard deviations for individual participants and for the group as a whole. A participant should be able to readily determine the level and variability of his results in comparison with those of the other laboratories.

Repeatability and Reproducibility Statements such as Contained in ASTM, TAPPI and ISO Standards are included at the end of the report. Participants can check their performance level against the precision statement given in the test method or specification.

TABLE OF CONTENTS

Analyses In This Report

PAGE

1	Introduction
11	Description of Program
iv	Metric Conversion Table
1	Key to Tables and Graphs
5	10-1 Bursting Strength - Up to 45 psi
8	10-2 Bursting Strength - Up to 45 psi, Air Clamps
11	11-1 Bursting Strength - Up to 100 psi
14	15-1 Tearing Strength - Deep Cutout
19	17-1 Tearing Strength - No Cutout
21	19-1 Tensile Breaking Strength - Packaging Papers
24	20-1 Tensile Breaking Strength - Printing Papers, CRE
27	20-2 Tensile Breaking Strength - Printing Papers, pendulum
30	25-1 Tensile Energy Absorption - Packaging Papers
32	26-1 Tensile Energy Absorption - Printing Papers
34	28-1 Elongation to Break - Packaging Papers
37	29-1 Elongation to Break - Printing Papers
40	30-1 Folding Endurance, MIT type
43	30-2 Folding Endurance, MIT type, log (base 10)
46	35-1 Stiffness, Gurley
49	36-1 Stiffness, Taber
52	49-1 Surface Pick Strength, IGT
54	50-1 Surface Pick Strength, Wax
57	91-1 Concora (Flat Crush)
59	96-1 Ring Crush
62	Summary

Diagram of Elmendorf tear testers, deep cutout vs. no cutout

Analyses In The G Report

40-1	Air Resistance, Gurley Oil type
40-2	Air Resistance, Sheffield type
41-1	Air Resistance, Gurley Mercury type
44-1	Smoothness, Parker Printsurf
45-1	Smoothness, Sheffield type
45-2	Smoothness, Bekk type
47-1	Smoothness, Bendtsen type
56-1	K & N Ink Absorption
57-1	pH, Cold Extraction
57-2	pH, Hot Extraction
60-1	Opacity, White (89%) Backing
60-2	Opacity, Paper Backing, B & L type
60-3	Opacity, Paper Backing, Elrepho type
65-1	Blue Reflectance (Brightness), Directional
65-2	Blue Reflectance, Diffuse, Elrepho (Gloss Trap)
65-3	Blue Reflectance, Diffuse, Elrepho (No Gloss Trap)
75-1	Specular Gloss, 75 degree
90-1	Thickness (Caliper)
95-1	Grammage (Basis Weight)

TABLE OF CONVERSION FACTORS TO METRIC (SI) UNITS

<u>Physical Quantity</u>	<u>To Convert From</u>	<u>To</u>	<u>Multiply by</u>
Bursting strength	psi	kPa	6.895
	kg/cm ²	kPa	98.07
	bar	kPa	100.00
Tearing strength	g	mN	9.807
Tensile strength	lb/in.	kN/m	.1751
	lb/0.5 in.	kN/m	.3502
	lb/15 mm	kN/m	.2965
	kg/15 mm	kN/m	.6538
	kg/25 mm	kN/m	.3923
	kg/mm	kN/m	9.807
Tensile energy absorption	ft-lb/ft ²	J/m ²	14.59
	in.-lb/in. ²	J/m ²	175.1
	kg-m/m ²	J/m ²	9.807
Bending stiffness	g·cm	μN·m	98.07
Flat-crush strength (Concora)	lb	N	4.448
Ring-crush (TAPPI)	lb	N	4.448
	(ISO)	lb/6.00 in.	kN/m
Thickness	mil	μm	25.40

KEY TO TABLES AND GRAPHS

- MEAN - The average of individual TEST DETERMINATIONS. The number of TEST DETERMINATIONS in the mean is given in the upper right corner of the first table (TEST D.) and again at the bottom of this table.
- GRAND MEAN - (GR. MEAN) The average of the individual laboratory MEANS, excluding laboratories flagged (see column F) with an X, #, or +. The GRAND MEAN is given in US customary units and, where applicable, in SI metric units.
- SD OF MEANS - (SD MEANS) The standard deviation of the laboratory MEANS about the GRAND MEAN; an index of the among-laboratory precision.
- DEV - The deviation or difference of the laboratory MEAN from the GRAND MEAN.
- N. DEV - The normal deviate or ratio of the DEV to the SD OF MEANS; an indication of the degree of divergence of the laboratory MEAN from the GRAND MEAN. A N. DEV of more than 2 or less than -2 may indicate that the participant is not following the procedure considered standard for this analysis.
- SDR - The standard deviation of repeated measurements; that is, of individual test determinations about their MEAN.
- AVERAGE SDR - The average of the individual laboratory SDR's; an index of the within-laboratory precision of repeated measurements.
- R. SDR - The relative standard deviation of repeated measurements; that is, the ratio of the SDR to the AVERAGE SDR: an indication of the ability of a participant to repeat his measurements relative to the average ability. The greater the number of TEST DETERMINATIONS the closer the R. SDR should be to unity. If R. SDR is outside the limits given below, the participant may not be following the procedure considered standard for this analysis:

<u>No. of test Determinations</u>	<u>Lower limit for R. SDR</u>	<u>Upper limit for R. SDR</u>
3	0.09	2.58
5	0.27	2.06
8	0.40	1.77
10	0.46	1.67
15	0.56	1.53
20	0.61	1.45
25	0.65	1.39

- VAR - Code for instrument type or variation in condition, see second table.
- F - Flag, with following meaning:
- + - Excluded from grand means because VAR non-standard for this analysis
 - # - Excluded because data were not understood or because of a non-coded variation reported by the laboratory. (See NOTES following Table 1 for each method.)
 - M - Excluded because data for one sample are missing
 - X - Excluded because plotted point would fall outside of the 99% error ellipse, (see below for explanation of Graph)
 - * - Included in grand means but plotted point falls outside of the 95% error ellipse. The participant should take this as a warning to reexamine his testing procedure
 - S - Included in grand mean but only after omission of one of more 'wild' values; that is, test determinations more than 3 times AVERAGE SDR from the laboratory's MEAN. Not more than 20% of the test determination may be excluded in this manner without rejecting the laboratory.
 - O - Included in grand mean and inside 95% error ellipse.
- COORDINATES - Distances along major and minor axes of error ellipse. If special additive or concurrent model of the measuring process applies to this method, the distance along the minor axis represents the random error within a laboratory while that along the major axis also includes a systematic laboratory component of error.

- 95% ELLIPSE - Lengths of the major and minor axes of the ellipse and the angle that the major axis makes with the horizontal axis.
- AVG R. SDR - Average of the R. SDR for the two samples; an indication of the laboratory's precision of repeated measurements.
- Graph - For each laboratory the MEAN for the second sample is plotted against the MEAN for the first sample, with each point representing a laboratory. The horizontal and vertical lines are the GRAND MEANS. The dashed line is drawn at 45°. The solid sloping line, which may or may not lie close to the 45° line, is along the major axis of the error ellipse. The ellipse is drawn so that , on the average, it will include 95% of the points representing the laboratories.

Plotted symbols are as explained above (under F), except that an 'S' is plotted as an 'O'. A participant whose plotted point falls outside of the ellipse should carefully reexamine the testing procedure he is following.

The graph is plotted with an ellipse when there are 20 or more laboratories in the analysis. When there are 10 through 19 laboratories in the analysis the graph is plotted but the ellipse is omitted. When there are fewer than 10 laboratories retained in the analysis the graph is not plotted.

The International System of Units (SI) is used on the plots wherever possible to aid participants in familiarizing themselves with SI. Grand means in SI units are given at the top of the plot, and supplementary scales in SI units are drawn along the axes allowing the reader to compare means and variability in common units and SI units for the same data.

- Summary - In addition to several quantities already defined above the summary shows the following values for each test method:
(At end of report)
- REPL CRP - The number of replicate test determinations used in this Collaborative Reference Program.
- REPL TAPPI - The number of replicate test determinations in a test result required by the applicable TAPPI Standard or assumed here if there is no TAPPI Standard. This quantity is needed in the computation of TAPPI repeatability and reproducibility from the SD OF MEANS and the AVER SDR. See TAPPI Standard T1206 for definitions and computations.
- REPEAT - TAPPI repeatability, a measure of the within-laboratory precision of a test result.
- REPROD - TAPPI reproducibility, a measure of the between-laboratory precision of a test result.
- Best values - Given at the end of Table 1 for each method for which sufficient information is available. These best values are estimates based on a careful examination of all data, both current and past, with special attention to results obtained by the National Bureau of Standards and other recognized reference laboratories in this and other countries. All participants using equipment that is standard for the analysis should be able to achieve results within the plus-minus (+) limits, when these are shown along with the best values.

TAPPI STANDARD T403 G9-76, BURSTING STRENGTH OF PAPER - PERKINS MODEL C

LAB CODE	SAMPLE H63 MEAN	PRINTING 77 GRAMS PER SQUARE METER				SAMPLE J39 MEAN	PRINTING 149 GRAMS PER SQUARE METER				TEST D. = 15		
		DEV	N. DEV	SDR	R. SDR		DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L121	16.89	.21	.16	.70	.67	26.80	-2.09	-0.99	1.52	1.03	10C	Ø	L121
L131	15.00	-1.69	-1.28	.76	.73	26.60	-2.29	-1.09	.91	.61	10C	Ø	L131
L134	16.40	-.29	-.22	.57	.55	32.37	3.48	1.65	1.17	.79	10C	*	L134
L150	17.67	.98	.74	1.18	1.13	29.27	.38	.18	.92	.62	10C	Ø	L150
L158	15.00	-.69	-.52	1.20	1.15	28.47	-.42	-.20	.92	.62	10C	Ø	L158
L167	17.43	.75	.56	.68	.65	28.00	-.89	-.42	1.20	.81	10C	Ø	L167
L183	15.57	-1.11	-.84	1.08	1.03	26.00	-2.89	-1.37	1.66	1.12	10C	Ø	L183
L191	16.73	.05	.03	.73	.70	30.00	1.11	.53	1.64	1.10	10C	Ø	L191
L203A	15.77	-.92	-.70	.82	.79	28.67	-.22	-.11	1.59	1.07	10C	Ø	L203A
L203B	16.47	-.22	-.17	.95	.92	29.57	.68	.32	2.27	1.53	10C	Ø	L203B
L207	19.20	2.51	1.90	1.19	1.14	32.10	3.21	1.52	1.84	1.24	10C	Ø	L207
L212	16.53	-.15	-.12	.74	.71	31.53	2.64	1.26	1.49	1.01	10C	Ø	L212
L223A	19.28	2.59	1.96	1.06	1.02	33.53	4.64	2.20	1.71	1.15	10C	Ø	L223A
L225	16.90	.21	.16	1.21	1.16	29.80	.91	.43	1.86	1.25	10C	Ø	L225
L222	14.60	-2.09	-1.58	1.07	1.03	27.27	-1.62	-.77	1.29	.87	10C	Ø	L222
L237A	15.73	-.95	-.72	.88	.85	26.37	-2.52	-1.20	1.30	.88	10C	Ø	L237A
L237B	16.33	-.35	-.27	.94	.90	27.10	-1.79	-.85	.60	.41	10C	Ø	L237B
L243	17.67	.98	.74	1.32	1.27	29.37	.48	.23	1.38	.93	10C	Ø	L243
L249	13.68	-3.01	-2.27	.79	.76	25.59	-3.30	-1.57	1.35	.91	10C	Ø	L249
L261	16.17	-.52	-.39	.82	.79	27.28	-1.61	-.76	1.66	1.12	10C	Ø	L261
L264	16.80	.11	.08	1.08	1.04	28.73	-.16	-.07	1.58	1.06	10C	Ø	L264
L278	16.90	.21	.16	1.02	.98	27.90	-.99	-.47	1.78	1.20	10C	Ø	L278
L279	15.73	-.95	-.72	1.57	1.50	27.10	-1.79	-.85	1.27	.85	10C	Ø	L279
L299	18.93	2.25	1.70	1.43	1.37	34.00	5.11	2.43	1.89	1.27	10C	Ø	L299
L305	16.63	-.05	-.04	1.03	.98	27.70	-1.19	-.56	.92	.62	10C	Ø	L305
L311	17.93	1.25	.94	.80	.77	30.07	1.18	.56	1.22	.82	10C	Ø	L311
L312	16.72	.03	.02	.89	.85	28.61	-.28	-.13	.88	.59	10C	Ø	L312
L315	18.73	2.05	1.55	1.31	1.25	31.57	2.68	1.27	1.85	1.25	10C	Ø	L315
L325	16.47	-.22	-.17	.88	.84	29.47	.58	.27	1.94	1.31	10C	Ø	L325
L330	17.90	1.21	.92	1.16	1.11	29.90	1.01	.48	1.39	.93	10C	Ø	L330
L331	16.33	-.35	-.27	1.05	1.00	27.13	-1.76	-.83	1.25	.84	10C	Ø	L331
L333	14.81	-1.88	-1.42	1.29	1.24	26.61	-2.28	-1.08	2.12	1.43	10C	Ø	L333
L339	12.88	-3.80	-2.88	1.40	1.34	25.13	-3.76	-1.78	1.51	1.02	10C	*	L339
L344	16.87	.19	.14	.90	.86	32.37	3.48	1.65	1.71	1.15	10C	Ø	L344
L356	17.50	.81	.61	1.26	1.21	26.91	-1.98	-.94	1.94	1.31	10C	Ø	L356
L358	16.23	-.45	-.34	.68	.65	29.64	.75	.36	1.16	.78	10C	Ø	L358
L360	16.73	.05	.03	1.54	1.48	28.69	-.20	-.10	1.92	1.30	10C	Ø	L360
L366	17.40	.71	.54	1.27	1.22	28.70	-.19	-.09	1.81	1.22	10C	Ø	L366
L390	18.27	1.58	1.19	1.07	1.02	30.47	1.58	.75	1.33	.90	10C	Ø	L390
L563	16.70	.01	.01	1.16	1.12	29.30	.41	.20	1.41	.95	10C	Ø	L563
L568	16.97	.28	.21	1.14	1.10	28.67	-.22	-.11	1.18	.79	10C	Ø	L568
L599	17.41	.72	.54	1.06	1.02	29.01	.12	.06	1.68	1.13	10C	Ø	L599

GR. MEAN = 16.69 PSI

SD MEANS = 1.32 PSI

GRAND MEAN = 28.89 PSI

SD OF MEANS = 2.11 PSI

TEST DETERMINATIONS = 15

42 LABS IN GRAND MEANS

AVERAGE SDR = 1.04 PSI

AVERAGE SDR = 1.48 PSI

GR. MEAN = 115.1 KILOPASCAL

GRAND MEAN = 199.2 KILOPASCAL

L128	18.33	1.65	1.24	.62	.59	30.53	1.64	.78	1.30	.88	10B	*	L128
L242	19.45	2.76	2.09	1.15	1.10	29.48	.59	.28	1.33	.90	10C	*	L242
L251	18.12	1.44	1.09	1.45	1.39	30.16	1.27	.60	1.22	.82	10V	*	L251
L269	24.47	7.78	5.88	1.55	1.49	37.40	8.51	4.04	1.80	1.22	10A	*	L269
L484	15.67	-1.02	-.77	.77	.74	26.50	-2.39	-1.13	1.21	.82	10M	*	L484

TOTAL NUMBER OF LABORATORIES REPORTING = 47

Best values: H63 16.8 ± 2.2 psi

J39 29.0 ± 3.4 psi

ANALYSIS T10=1 TABLE 2


BURSTING STRENGTH, PSI

TAPPI STANDARD T403 GS=76, BURSTING STRENGTH OF PAPER = PERKINS MODEL C

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY==TEST	INSTRUMENT==CONDITIONS
		H63	J39	MAJOR	MINOR	R.SDR	VAR		
L335	*	12.88	25.13	-5.11	1.55	1.18	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L249	0	13.68	25.59	-4.34	1.07	.83	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L232	0	14.60	27.27	-2.42	1.06	.95	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L333	0	14.81	26.61	-2.90	.57	1.33	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L131	0	15.00	26.60	-2.82	.39	.67	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L183	0	15.57	26.00	-3.07	-0.40	1.08	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L484	*	15.67	26.50	-2.59	-0.24	.78	10M	BURSTING STRENGTH UP T0 45 PSI, REGMED MT/MOT,	MANUAL CLAMP
L279	0	15.73	27.10	-2.03	-0.01	1.18	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L237A	0	15.73	26.37	-2.67	-0.36	.86	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L203A	0	15.77	28.67	-0.63	.70	.93	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L158	0	16.00	28.47	-0.70	.40	.88	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L261	0	16.17	27.28	-1.66	-0.31	.95	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L358	0	16.23	29.64	.44	.76	.72	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L331	0	16.33	27.13	-1.71	-0.53	.92	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L237B	0	16.33	27.10	-1.74	-0.54	.65	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L134	*	16.40	32.37	2.92	1.91	.67	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L326	0	16.47	29.47	.40	.47	1.07	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L203B	0	16.47	29.57	.49	.52	1.22	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L212	0	16.53	31.53	2.25	1.40	.86	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L305	0	16.63	27.70	-1.07	-0.52	.80	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L563	0	16.70	29.30	.37	.19	1.03	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L312	0	16.72	28.61	-0.23	-0.16	.72	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L360	0	16.73	28.69	-0.16	-0.14	1.39	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L291	0	16.73	30.00	1.00	.49	.90	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L264	0	16.80	28.73	-0.08	-0.17	1.05	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L344	0	16.87	32.37	3.15	1.49	1.01	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L121	0	16.89	26.80	-1.74	-1.18	.85	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L278	0	16.90	27.90	-0.77	-0.66	1.09	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L225	0	16.90	29.80	.90	.25	1.21	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L568	0	16.97	28.67	-0.06	-0.35	.94	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L366	0	17.40	28.70	.17	-0.72	1.22	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L599	0	17.41	29.01	.45	-0.58	1.07	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L167	0	17.43	28.00	-0.43	-1.08	.73	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L356	0	17.50	26.91	-1.36	-1.66	1.26	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L150	0	17.67	29.27	.80	-0.66	.88	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L243	0	17.67	29.37	.89	-0.63	1.10	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L330	0	17.90	29.90	1.47	-0.58	1.02	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L311	0	17.93	30.07	1.63	-0.53	.80	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L251	*	18.12	30.16	1.80	-0.66	1.11	10V	BURSTING STRENGTH UP T0 45 PSI, L*W, MANUAL CLAMP, 20C, 65% RH	
L390	0	18.27	30.47	2.14	-0.64	.96	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L128	*	18.33	30.53	2.23	-0.66	.74	10B	BURSTING STRENGTH UP T0 45 PSI, PERKINS B,	MANUAL CLAMP
L315	0	18.73	31.57	3.33	-0.52	1.25	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L299	0	18.93	34.00	5.56	.46	1.32	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L207	0	19.20	32.10	4.02	-0.68	1.19	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L223A	0	19.28	33.53	5.32	-0.67	1.09	10C	BURSTING STRENGTH UP T0 45 PSI, PERKINS C,	MANUAL CLAMP
L242	*	19.45	29.48	1.84	-2.14	1.00	10T	BURSTING STRENGTH UP T0 45 PSI, L*W, MANUAL CLAMP	
L269	*	24.47	37.40	11.19	-2.78	1.35	10A	BURSTING STRENGTH UP T0 45 PSI, PERKINS A,	MANUAL CLAMP
GMEANS:		16.69	28.89			1.00			
		95% ELLIPSE:		6.07	2.05	WITH GAMMA = 61 DEGREES			

BURSTING STRENGTH, MODEL C

SAMPLE H63 = 16.7 PSI SAMPLE J39 = 28.9 PSI
 SAMPLE H63 = 115 KILOPASCAL SAMPLE J39 = 199 KILOPASCAL

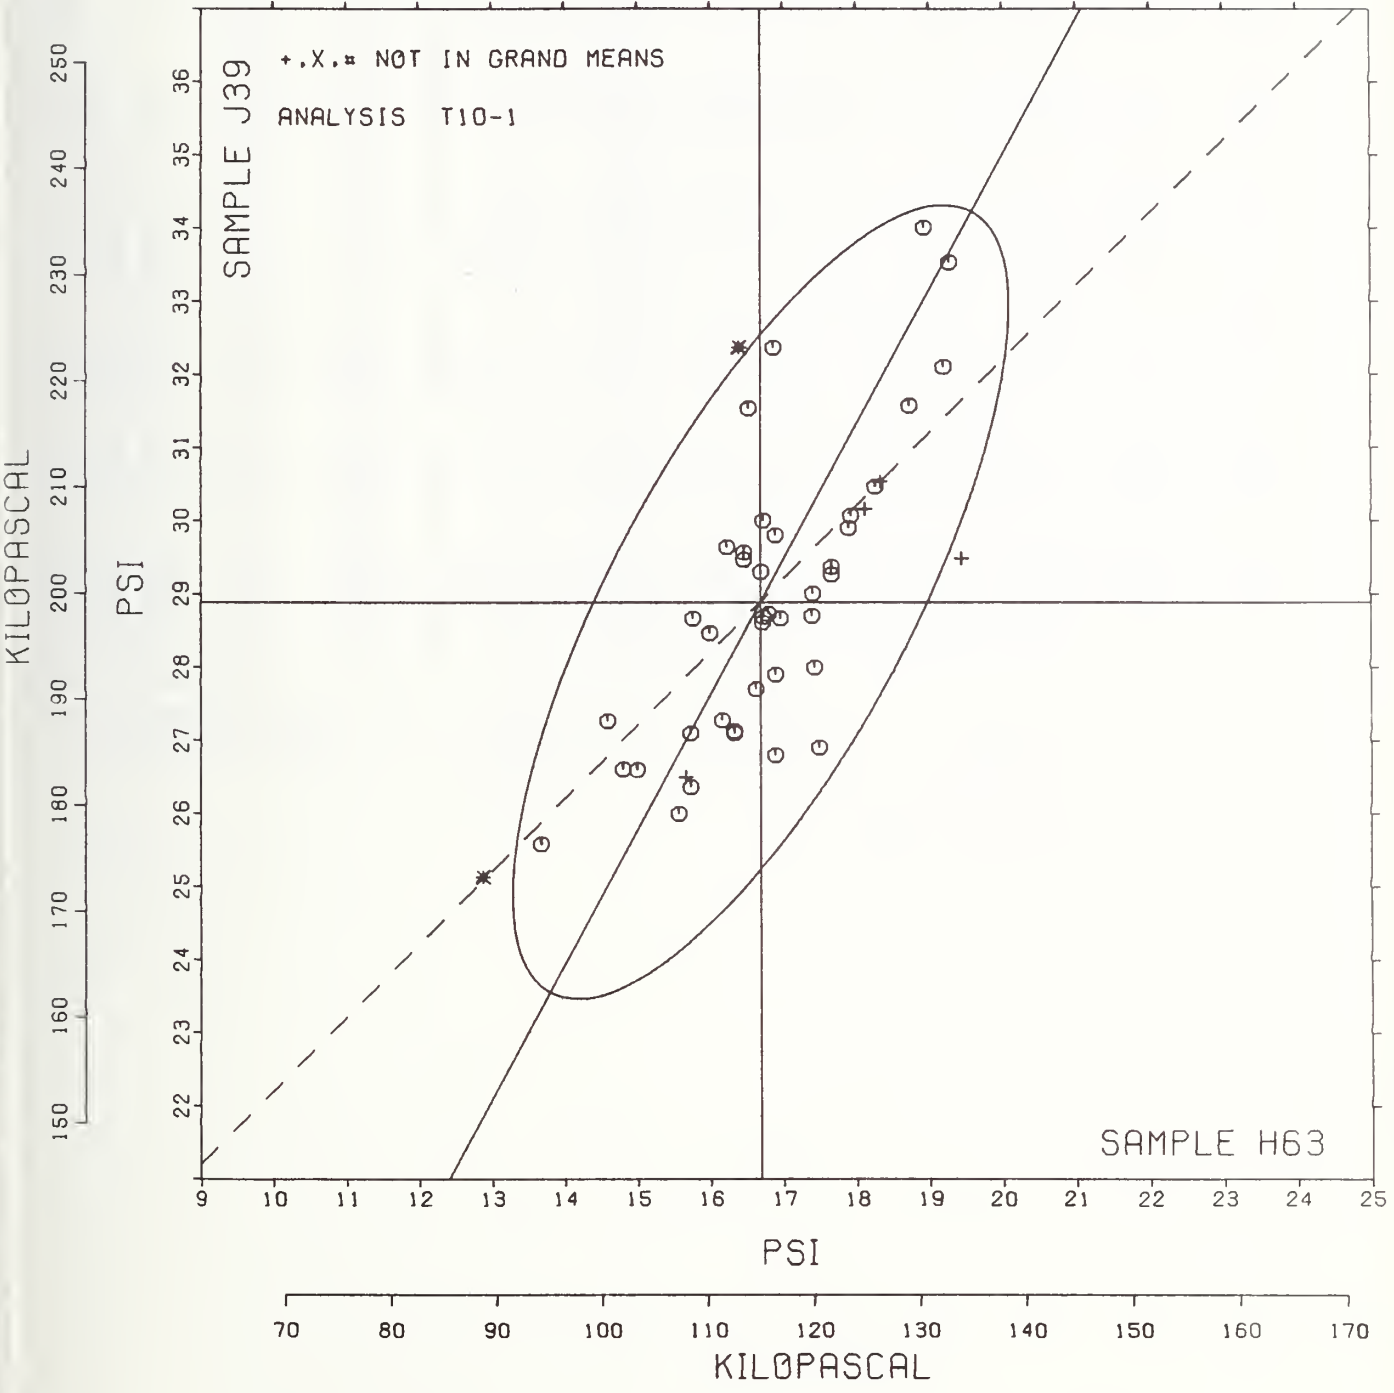

TAPPI STANDARD T403 6S-76, BURSTING STRENGTH OF PAPER - PERKINS MODEL C-A OR C WITH AIR OR HYDRAULIC CLAMPS

LAB CODE	SAMPLE H63		PRINTING 77 GRAMS PER SQUARE METER				SAMPLE J39		PRINTING 149 GRAMS PER SQUARE METER				TEST D. = 15		
	MEAN	DEV	N. DEV	SDR	R. SDR	MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB		
L100	17.79	1.13	.69	.85	.74	29.05	.35	.18	1.37	.93	10D	0	L100		
L105	12.67	-3.99	-2.46	.86	.75	24.37	-4.33	-2.25	1.66	1.13	10D	0	L105		
L122	17.73	1.08	.66	1.03	.90	30.80	2.10	1.09	.56	.38	10F	0	L122		
L125	13.40	-3.26	-2.01	1.64	1.43	24.80	-3.90	-2.02	2.24	1.52	10D	0	L125		
L141	16.57	-.09	-.06	1.39	1.21	28.20	-.50	-.26	1.80	1.22	10D	0	L141		
L148	17.87	1.21	.74	.92	.80	28.53	-.17	-.09	1.73	1.17	10D	0	L148		
L159	15.41	-1.25	-.77	1.19	1.04	27.55	-1.15	-.60	1.23	.84	10D	0	L159		
L162	15.47	-1.19	-.73	.74	.65	27.13	-1.57	-.81	1.77	1.20	10D	0	L162		
L163	16.63	-.02	-.02	1.04	.91	28.80	.10	.05	1.84	1.25	10D	0	L163		
L166	15.37	-.29	-.18	1.53	1.34	29.17	.47	.24	1.81	1.02	10D	0	L166		
L176	19.32	2.68	1.65	.62	.54	30.13	1.43	.74	1.19	.81	10D	0	L176		
L185	18.00	1.34	.83	.76	.66	31.00	2.30	1.19	1.77	1.21	10D	0	L185		
L190C	15.97	-.69	-.43	1.52	1.33	28.37	-.33	-.17	.93	.64	10D	0	L190C		
L217	17.67	1.01	.62	.82	.71	28.67	-.03	-.02	1.35	.91	10P	0	L217		
L224	17.23	.58	.35	1.40	1.23	29.07	.37	.19	1.46	.99	10D	0	L224		
L226B	17.71	1.05	.65	1.06	.93	28.98	.28	.14	1.42	.96	10D	0	L226B		
L226C	14.37	-2.29	-1.41	1.04	.91	26.53	-2.17	-1.12	1.76	1.19	10D	0	L226C		
L255	16.20	-.46	-.28	.77	.68	26.67	-2.03	-1.05	.72	.49	10D	0	L255		
L257A	17.60	.94	.58	1.30	1.14	31.60	2.90	1.50	2.13	1.45	10D	0	L257A		
L257B	17.13	.48	.29	1.41	1.23	31.60	2.90	1.50	1.30	.88	10D	0	L257B		
L257C	17.60	.94	.58	1.30	1.14	32.00	3.30	1.71	1.65	1.12	10D	0	L257C		
L262	17.57	.91	.56	1.05	.92	30.60	1.90	.98	1.53	1.04	10D	0	L262		
L275	13.88	-2.78	-1.71	1.33	1.16	26.29	-2.41	-1.25	1.73	1.18	10D	0	L275		
L280	18.26	1.60	.99	.88	.77	29.73	1.03	.53	1.00	.68	10D	0	L280		
L285	16.60	-.66	-.04	1.55	1.36	29.47	.77	.40	1.51	1.02	10D	0	L285		
L309	13.73	-2.93	-1.81	1.27	1.11	26.57	-2.13	-1.10	1.39	.95	10D	0	L309		
L352	16.50	-.16	-.10	.86	.75	26.54	-2.16	-1.12	1.18	.80	10D	0	L352		
L378	18.07	1.41	.87	1.44	1.26	28.67	-.03	-.02	1.54	1.05	10D	0	L378		
L575	18.51	1.85	1.14	1.68	1.47	28.93	.23	.12	1.71	1.16	10D	0	L575		
L581	17.67	1.01	.62	1.45	1.27	29.13	.43	.22	1.55	1.06	10D	0	L581		
L587	16.93	.28	.17	.73	.64	30.77	2.07	1.07	1.08	.74	10D	0	L587		

GR. MEAN = 16.66 PSI
SD MEANS = 1.62 PSI

GRAND MEAN = 28.70 PSI
SD OF MEANS = 1.93 PSI

TEST DETERMINATIONS = 15
31 LABS IN GRAND MEANS

GR. MEAN = 114.9 KILOPASCAL

AVERAGE SDR = 1.14 PSI

AVERAGE SDR = 1.47 PSI

GRAND MEAN = 197.9 KILOPASCAL

L442 145.33 128.67 79.25 20.14 17.63 281.27 252.57 130.85 44.50 30.25 10Q * L442
TOTAL NUMBER OF LABORATORIES REPORTING = 32

Best values: H63 17.0 ± 2.8 psi
J39 28.9 ± 2.6 psi

TAPPI STANDARD T403 69-76, BURSTING STRENGTH OF PAPER - PERKINS MODEL C-A OR C WITH AIR OR HYDRAULIC CLAMPS

LAB CODE	P	MEANS		COORDINATES		AVG		PROPERTY---	TEST	INSTRUMENT---	CONDITIONS
		H63	J39	MAJOR	MINOR	R.SDR	VAR				
L105	Ø	12.67	24.37	-5.88	.39	.94	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L125	Ø	13.40	24.80	-5.08	.09	1.48	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L309	Ø	13.73	26.57	-3.49	.95	1.03	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L275	Ø	13.88	26.29	-3.62	.66	1.17	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L226C	Ø	14.37	26.53	-3.13	.43	1.05	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L159	Ø	15.41	27.55	-1.68	.25	.94	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L162	Ø	15.47	27.13	-1.97	-.05	.93	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L190C	Ø	15.97	28.37	-.69	.33	.98	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L255	Ø	16.20	26.67	-1.87	-.92	.59	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L166	Ø	16.37	29.17	.18	.52	1.18	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L352	Ø	16.50	26.54	-1.78	-1.23	.78	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L141	Ø	16.57	28.20	-.45	-.24	1.22	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L285	Ø	16.60	29.47	.56	.53	1.19	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L163	Ø	16.63	28.80	.06	.08	1.08	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L587	Ø	16.93	30.77	1.78	1.08	.69	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L257B	Ø	17.13	31.60	2.56	1.45	1.06	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L224	Ø	17.23	29.07	.65	-.22	1.11	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L262	Ø	17.57	30.60	2.05	.48	.98	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L257C	Ø	17.60	32.00	3.16	1.33	1.13	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L257A	Ø	17.60	31.60	2.85	1.08	1.29	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L581	Ø	17.67	29.13	.97	-.51	1.16	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L217	Ø	17.67	28.67	.61	-.81	.81	10F	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS C, H ₂ O CLAMP, TRANSDUCER
L226B	Ø	17.71	28.98	.87	-.64	.95	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L122	Ø	17.73	30.80	2.31	.48	.64	10F	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS C, H ₂ O CLAMP, TRANSDUCER
L100	Ø	17.79	29.05	.98	-.66	.84	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L148	Ø	17.87	28.53	.63	-1.05	.99	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L185	Ø	18.00	31.00	2.63	.40	.93	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L378	Ø	18.07	28.67	.86	-1.12	1.15	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L280	Ø	18.26	29.73	1.81	-.60	.73	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L575	Ø	18.51	28.93	1.34	-1.29	1.32	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L176	Ø	19.33	30.13	2.79	-1.19	.67	10D	BURSTING	STRENGTH	UP TØ 45 PSI,	PERKINS CA ØR C, AIR CLAMP
L442	*	145.33	281.27	277.46	58.00	23.94	10Q	BURSTING	STRENGTH	UP TØ 45 PSI,	FRANK, HYD. CL.
GMEANS:		16.66	28.70			1.00					
		95% ELLIPSE:		6.28	2.10	WITH GAMMA = 51 DEGREES					


BURSTING STRENGTH, MODEL C-A

SAMPLE H63 = 16.7 PSI

SAMPLE J39 = 28.7 PSI

SAMPLE H63 = 115 KILOPASCAL

SAMPLE J39 = 198 KILOPASCAL

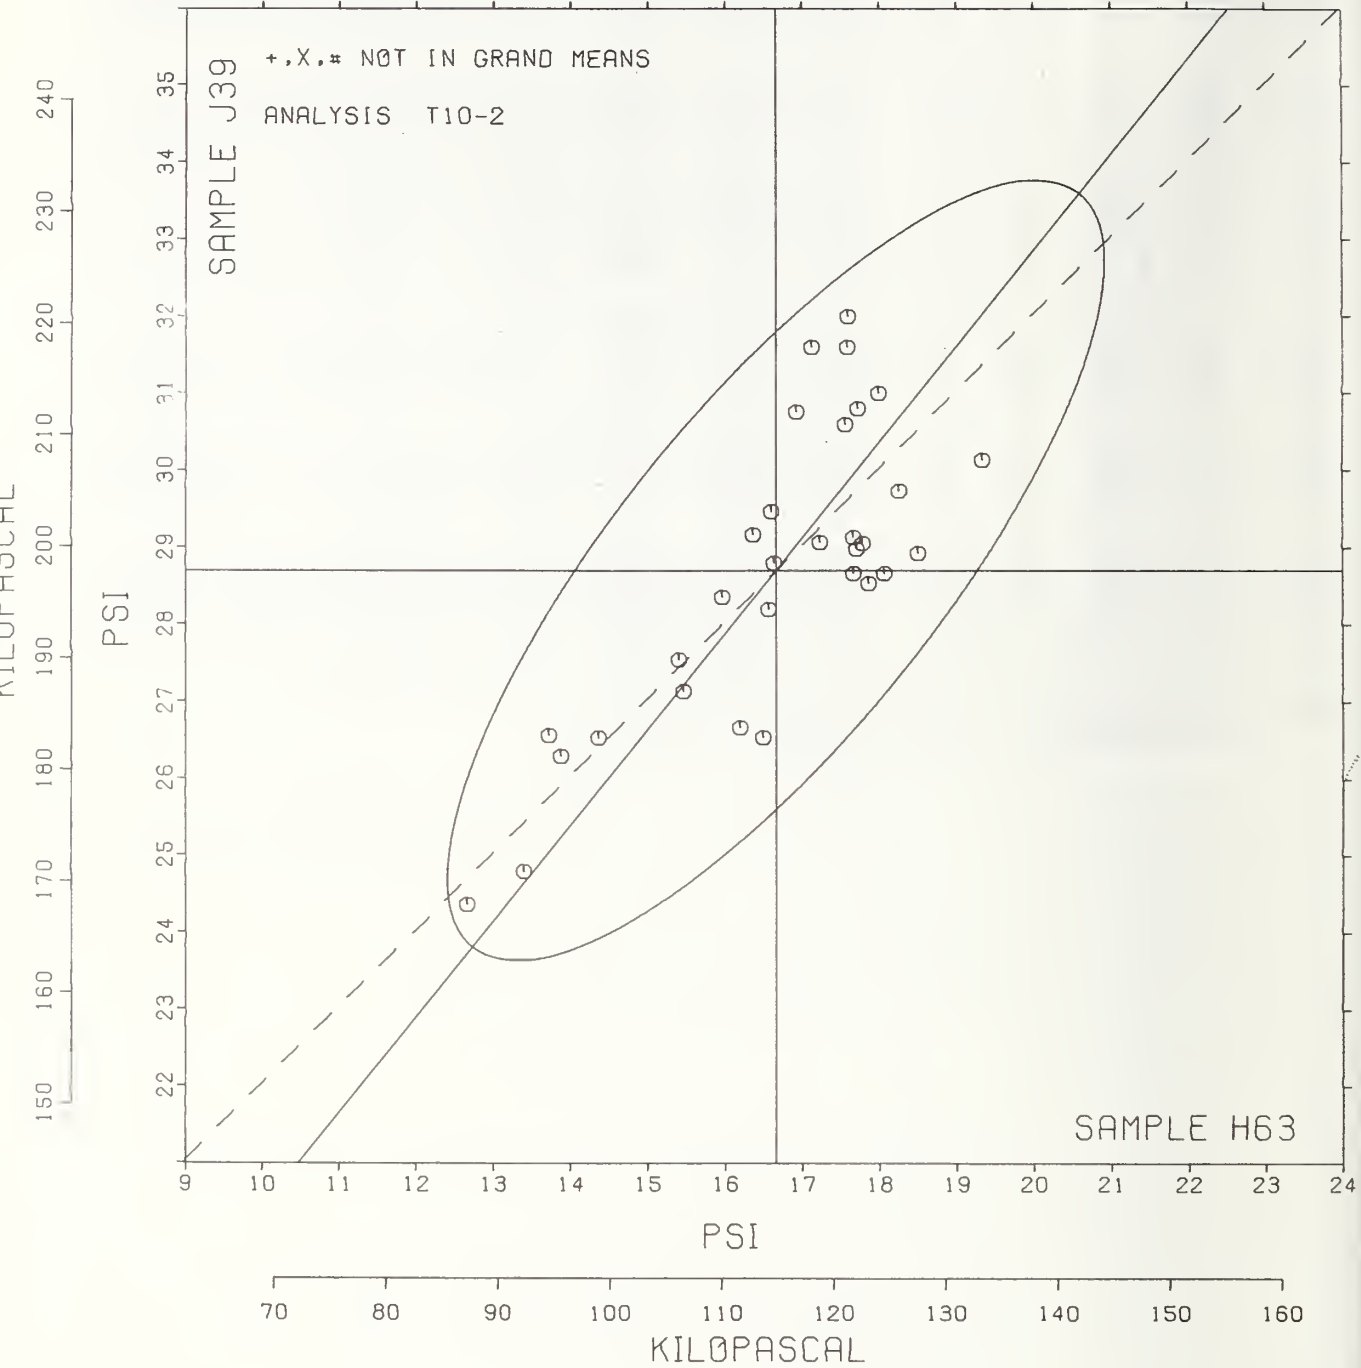

ANALYSIS T11-1 TABLE 1
BURSTING STRENGTH, HIGH RANGE, PSI
TAPPI STANDARD T403 CS-76, BURSTING STRENGTH OF PAPER - PERKINS MODEL C OR C-A

LAB CODE	SAMPLE E77 MEAN	TUBE WINDING 132 GRAMS PER SQUARE METER				R. SDR	SAMPLE K29 MEAN	KRAFT 123 GRAMS PER SQUARE METER				TEST D. = 15		
		DEV	N. DEV	SDR	R. SDR			DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L100	69.5	-5.1	-1.57	4.4	.88	59.3	-0.1	-0.03	2.6	.63	11D	0	L100	
L103	74.9	.3	.09	4.4	.88	63.3	3.9	1.59	2.9	.70	11C	0	L103	
L107	80.1	5.5	1.70	4.1	.82	63.7	4.3	1.74	4.9	1.20	11C	0	L107	
L122	73.1	-1.5	-0.45	5.4	1.10	58.9	-0.5	-0.21	5.1	1.23	11F	0	L122	
L128	71.7	-2.9	-0.90	3.8	.76	59.1	-0.3	-0.11	2.2	.54	11D	0	L128	
L141	74.1	-0.5	-0.15	5.7	1.16	61.2	1.8	.72	5.3	1.29	11D	0	L141	
L148	75.8	1.2	.37	4.3	.87	60.9	1.5	.60	4.6	1.11	11D	0	L148	
L159	73.0	-1.6	-0.48	7.4	1.49	54.5	-4.9	-1.97	4.4	1.08	11D	0	L159	
L170	80.2	5.6	1.73	3.4	.68	61.3	1.9	.79	1.7	.41	11C	0	L170	
L176	78.6	4.0	1.23	5.6	1.13	59.5	.1	.06	3.9	.96	11D	0	L176	
L182	75.9	1.3	.39	6.2	1.25	61.3	1.9	.76	5.7	1.38	11D	0	L182	
L218	77.7	3.1	.96	6.1	1.23	60.8	1.4	.57	5.2	1.27	11D	0	L218	
L232	61.3	-13.3	-4.10	8.2	1.65	43.2	-16.2	-6.59	9.9	2.41	11C	#	L232	
L237A	73.6	-1.0	-0.32	1.9	.39	61.4	2.0	.80	3.1	.77	11C	0	L237A	
L237B	72.4	-2.2	-0.68	1.5	.29	60.2	.8	.31	2.5	.60	11C	0	L237B	
L238A	78.3	3.7	1.14	7.1	1.44	59.2	-0.2	-0.10	4.4	1.06	11Y	0	L238A	
L243	72.8	-1.8	-0.55	3.9	.79	59.4	.0	.00	4.1	1.01	11C	0	L243	
L278	72.8	-1.8	-0.56	5.0	1.01	57.9	-1.5	-0.62	4.5	1.11	11C	0	L278	
L279	72.1	-2.5	-0.77	5.0	1.01	57.2	-2.2	-0.89	5.6	1.36	11C	0	L279	
L280	73.4	-1.2	-0.38	4.5	.91	58.3	-1.1	-0.46	4.8	1.18	11D	0	L280	
L303	70.6	-4.0	-1.22	5.4	1.09	56.2	-3.2	-1.30	3.1	.75	11C	0	L303	
L330	74.7	.1	.02	6.9	1.39	60.6	1.2	.49	4.8	1.16	11C	0	L330	
L331	71.1	-3.5	-1.07	5.5	1.10	55.9	-3.5	-1.43	3.1	.75	11C	0	L331	
L333	78.3	3.7	1.12	5.9	1.19	61.3	1.9	.79	3.7	.90	11C	0	L333	
L344	72.0	-2.6	-0.81	2.7	.54	60.3	.9	.35	2.8	.69	11C	0	L344	
L356	72.7	-1.9	-0.58	5.0	1.01	58.4	-1.0	-0.40	5.6	1.37	11C	0	L356	
L362	67.9	-6.7	-2.07	6.0	1.21	55.0	-4.4	-1.78	5.0	1.22	11D	0	L362	
L378	77.8	3.2	.98	4.4	.88	60.0	.6	.25	3.6	.88	11D	0	L378	
L565	71.8	-2.8	-0.87	2.8	.57	59.8	.4	.16	1.8	.45	11D	0	L565	
L575	79.0	4.4	1.34	6.2	1.26	61.2	1.8	.71	4.8	1.18	11D	0	L575	
L581	74.9	.3	.08	4.3	.87	56.6	-2.8	-1.13	4.8	1.17	11D	0	L581	
L599	75.3	.7	.22	4.8	.96	57.9	-1.5	-0.59	4.1	1.00	11C	0	L599	
L604	76.2	1.6	.49	7.1	1.43	59.3	-0.1	-0.04	5.8	1.43	11C	0	L604	
L622	75.9	1.3	.39	5.8	1.18	56.8	-2.6	-1.06	3.6	.88	11E	0	L622	
L650	71.6	-3.0	-0.92	6.2	1.24	56.4	-3.0	-1.22	5.2	1.27	11D	0	L650	
L651	81.5	6.9	2.11	8.0	1.61	65.9	6.5	2.66	6.6	1.62	11D	*	L651	
GR. MEAN = 74.6 PSI		AVERAGE SDR = 5.0 PSI				GRAND MEAN = 59.4 PSI		AVERAGE SDR = 4.1 PSI				TEST DETERMINATIONS = 15		
SD MEANS = 3.3 PSI						SD OF MEANS = 2.5 PSI						35 LABS IN GRAND MEANS		
GR. MEAN = 514.4 KILOPASCAL						GRAND MEAN = 409.5 KILOPASCAL								
L242	76.3	1.7	.53	4.5	.91	61.9	2.5	1.02	6.2	1.51	11T	*	L242	
L251	69.6	-5.0	-1.52	6.8	1.38	55.9	-3.5	-1.41	4.1	1.00	11V	*	L251	
L393	73.4	-1.2	-0.37	5.6	1.13	58.8	-0.6	-0.24	2.9	.72	11E	*	L393	
L394	88.0	13.4	4.12	6.6	1.34	70.5	11.1	4.50	3.8	.92	11H	*	L394	
L484	82.0	7.4	2.27	2.3	.46	68.5	9.1	3.71	1.6	.39	11H	*	L484	
L570	78.7	4.1	1.25	6.6	1.32	64.9	5.5	2.22	3.9	.95	11H	*	L570	
L576	79.8	5.2	1.61	6.1	1.23	64.5	5.1	2.09	5.8	1.41	11P	*	L576	
L593	89.5	14.9	4.57	8.5	1.71	74.3	14.9	6.04	5.6	1.36	11J	*	L593	
L598	80.4	5.8	1.78	6.7	1.34	67.2	7.8	3.17	6.4	1.55	11*	*	L598	

TOTAL NUMBER OF LABORATORIES REPORTING = 45

Best values: E77 74 ± 5 psi
K29 59 ± 4 psi

The following laboratories were omitted from the grand means because of extreme test results: 232

ANALYSIS T11-1 TABLE 2

BURSTING STRENGTH, HIGH RANGE, PSI

TAPPI STANDARD T403 GS=76, BURSTING STRENGTH OF PAPER = PERKINS MODEL C OR C-A

LAB CODE	P	MEANS		COORDINATES		AVG R.SDR	VAR	PROPERTY	TEST	INSTRUMENT	CONDITIONS
		E77	K29	MAJOR	MINOR						
L232	#	61.3	43.2	-20.1	-6.3	2.03	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L362	Ø	67.9	55.0	-8.0	.0	1.21	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L100	Ø	69.5	59.3	-4.3	2.7	.75	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L251	*	69.6	55.9	-6.1	-2	1.19	11V	BURSTING	STRENGTH	40 = 100 PSI,	L*W, MANUAL CLAMP, 20C, 65% RH
L303	Ø	70.6	56.2	-5.1	-5	.92	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L331	Ø	71.1	55.9	-4.8	-1.0	.93	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L650	Ø	71.6	56.4	-4.2	-9	1.25	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L128	Ø	71.7	59.1	-2.6	1.4	.65	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L565	Ø	71.8	59.8	-2.2	1.9	.51	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L344	Ø	72.0	60.3	-1.7	2.2	.61	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L279	Ø	72.1	57.2	-3.3	-5	1.19	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L237B	Ø	72.4	60.2	-1.4	1.9	.45	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L356	Ø	72.7	58.4	-2.1	.2	1.19	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L278	Ø	72.8	57.9	-2.3	-3	1.06	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L243	Ø	72.8	59.4	-1.5	1.0	.90	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L159	Ø	73.0	54.5	-4.0	-3.2	1.28	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L122	Ø	73.1	58.9	-1.5	.4	1.17	11F	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, B. CLAMP, TRANSDUCER
L280	Ø	73.4	58.3	-1.6	-3	1.04	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L393	*	73.4	58.8	-1.3	.2	.92	11H	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS AB, HYDRAULIC CLAMP
L237A	Ø	73.6	61.4	.2	2.2	.58	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L141	Ø	74.1	61.2	.6	1.7	1.22	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L330	Ø	74.7	60.6	.7	1.0	1.28	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L581	Ø	74.9	56.6	-1.3	-2.5	1.02	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L103	Ø	74.9	63.3	2.4	3.1	.79	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L599	Ø	75.3	57.9	-2	-1.6	.98	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L148	Ø	75.8	60.9	1.8	.6	.99	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L182	Ø	75.9	61.3	2.1	.9	1.32	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L622	Ø	75.9	56.8	-4	-2.9	1.03	11E	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L604	Ø	76.2	59.3	1.3	-1.0	1.43	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L242	*	76.3	61.9	2.8	1.2	1.21	11T	BURSTING	STRENGTH	40 = 100 PSI,	L*W, MANUAL CLAMP
L218	Ø	77.7	60.8	3.4	-5	1.25	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L378	Ø	77.8	60.0	3.0	-1.2	.88	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L333	Ø	78.3	61.3	4.1	-4	1.04	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L238A	Ø	78.3	59.2	3.0	-2.2	1.25	11Y	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L176	Ø	78.6	59.5	3.4	-2.1	1.04	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L570	*	78.7	64.9	6.4	2.4	1.14	11H	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS AB, HYDRAULIC CLAMP
L575	Ø	79.0	61.2	4.6	-9	1.22	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L576	*	79.8	64.5	7.2	1.4	1.32	11P	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS LC, MANUAL CLAMP
L107	Ø	80.1	63.7	7.0	.5	1.01	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L170	Ø	80.2	61.3	5.8	-1.5	.55	11C	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS C, MANUAL CLAMP
L598	*	80.4	67.2	9.1	3.4	1.45	11*	BURSTING	STRENGTH	40 = 100 PSI,	MESSMER, MANUAL CLAMP
L651	*	81.5	65.9	9.3	1.7	1.61	11D	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS CA, AIR CLAMP
L484	*	82.0	68.5	11.2	3.6	.42	11H	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS AB, HYDRAULIC CLAMP
L394	*	88.0	70.5	17.3	1.9	1.13	11H	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS AB, HYDRAULIC CLAMP
L593	*	89.5	74.3	20.6	4.3	1.53	11J	BURSTING	STRENGTH	40 = 100 PSI,	PERKINS JUMBO, HAND DRIVEN
GMBANS:		74.6	59.4			1.00					
		95% ELLIPSE:		9.7	4.2			WITH GAMMA = 33 DEGREES			


BURSTING STRENGTH, HIGH RANGE

SAMPLE E77 = 74.6 PSI

SAMPLE K29 = 59.4 PSI

SAMPLE E77 = 514 KILOPASCAL

SAMPLE K29 = 410 KILOPASCAL

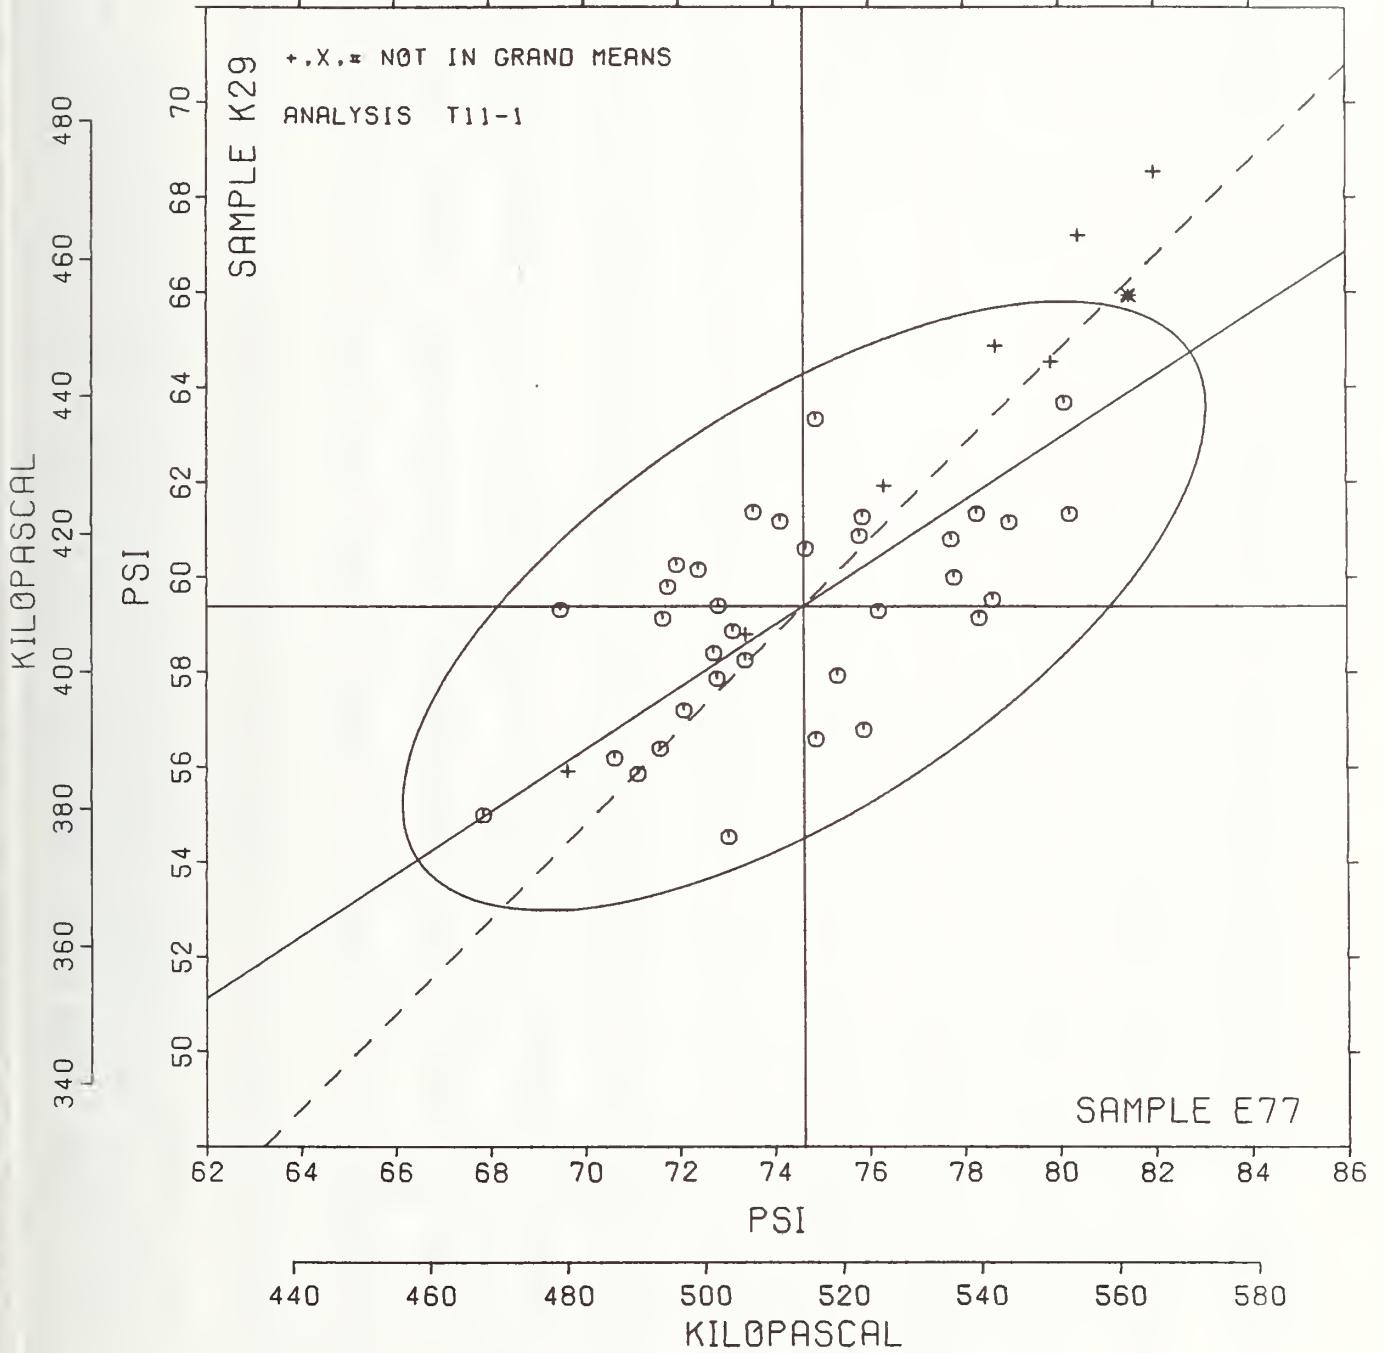

TAPPI STANDARD T414 TS-65, ANY MAKE BLEND OR P WITH DEEP CUTOUT IS STANDARD FOR THIS ANALYSIS

LAB CODE	SAMPLE E76 116 GRAMS PER SQUARE METER					SAMPLE E80 69 GRAMS PER SQUARE METER					TEST D. = 15		
	MEAN	DEV	N. DEV	SDR	R. SDR	MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L100	64.5	-1.4	0.36	2.6	1.01	53.9	-3.8	-1.03	1.0	.68	15M	0	L100
L103	82.1	-3.7	0.98	1.5	.60	55.1	-2.5	0.68	.9	.62	15T	0	L103
L105	84.6	-1.3	0.34	3.3	1.31	55.1	-2.5	0.68	1.1	.72	15T	0	L105
L107	88.5	2.7	.69	4.7	1.88	65.6	8.0	2.16	9.7	6.55	15T	*	L107
L121	82.9	-2.9	0.77	3.0	1.19	57.9	.2	.06	1.2	.81	15T	0	L121
L122	60.6	-5.3	-1.38	2.3	.93	54.1	-3.5	0.95	1.0	.68	15C	0	L122
L124	87.6	1.7	.45	3.3	1.31	60.3	2.6	.71	.7	.48	15T	0	L124
L126	88.3	2.4	.62	2.3	.93	59.1	1.4	.39	2.2	1.46	15T	0	L126
L128	84.9	0.9	0.25	1.5	.59	56.0	-1.6	0.45	1.7	1.15	15T	0	L128
L131	82.1	-3.7	0.98	5.0	1.98	54.9	-2.7	0.74	1.8	1.24	15A	0	L131
L134	86.3	.5	.12	2.1	.83	56.7	0.9	0.25	1.0	.65	15C	0	L134
L139	92.1	6.3	1.63	1.6	.65	63.8	6.2	1.67	1.7	1.15	15T	0	L139
L141	85.9	.1	.01	3.1	1.22	57.6	0.0	0.01	.8	.56	15T	0	L141
L143	67.5	1.6	.41	4.1	1.61	57.7	.0	.01	2.8	1.88	15T	0	L143
L145	82.1	-3.7	0.98	2.8	1.10	72.7	15.0	4.08	1.8	1.22	15T	#	L145
L148	84.8	-1.1	0.28	3.1	1.23	65.1	7.4	2.01	1.7	1.13	15T	*	L148
L150	87.9	2.1	.54	2.6	1.02	57.9	.3	.08	1.2	.79	15T	0	L150
L151	93.7	7.8	2.03	2.7	1.08	66.0	8.4	2.27	1.6	1.09	15C	0	L151
L158	82.3	-3.6	0.94	4.9	1.96	58.4	.8	.20	2.2	1.47	15R	0	L158
L159	67.7	1.9	.48	3.0	1.18	58.0	.4	.10	2.7	1.83	15L	0	L159
L162	87.1	1.2	.31	2.5	.99	57.6	0.0	0.01	1.1	.76	15T	0	L162
L163	64.9	-1.0	0.27	2.8	1.12	57.5	0.2	0.05	1.8	1.20	15T	0	L163
L166	88.7	2.8	.73	2.5	.98	58.2	.6	.15	1.4	.93	15T	0	L166
L167	85.3	0.5	0.14	1.0	.39	60.7	3.0	.82	1.0	.66	15C	0	L167
L170	83.5	-2.3	0.61	.9	.36	54.4	-3.2	0.88	.8	.56	15T	0	L170
L173B	84.8	-1.1	0.28	1.7	.66	61.6	4.0	1.07	1.1	.76	15T	0	L173B
L176	87.9	2.0	.52	2.3	.92	58.0	.4	.10	1.7	1.15	15T	0	L176
L182A	79.1	-6.7	-1.76	3.9	1.55	52.3	-5.4	-1.46	1.3	.87	15A	0	L182A
L182T	90.3	4.4	1.15	3.2	1.29	60.1	2.5	.67	1.2	.85	15T	0	L182T
L183	87.1	1.2	.31	2.8	1.12	56.1	-1.5	0.41	.6	.43	15T	0	L183
L185	87.5	-2.3	0.61	2.6	1.03	58.1	.5	.13	1.4	.92	15T	0	L185
L189	86.2	.3	.08	2.6	1.03	56.2	-1.4	0.39	1.2	.82	15T	0	L189
L190C	84.6	-1.3	0.34	2.5	.59	58.3	.6	.17	1.7	1.13	15T	0	L190C
L190R	85.1	.2	.05	2.4	.95	56.9	0.7	0.19	1.6	1.07	15C	0	L190R
L191	79.4	-6.5	-1.69	2.4	.95	51.0	-6.6	-1.80	2.5	1.70	15T	0	L191
L195	89.5	3.6	.94	2.6	1.02	56.1	-1.5	0.41	1.2	.81	15C	0	L195
L206	68.9	3.0	.79	1.9	.75	60.3	2.6	.72	1.8	1.22	15R	0	L206
L207	74.4	-11.5	-2.99	1.6	.65	47.1	-10.5	-2.85	2.5	1.67	15R	*	L207
L211	83.7	-2.1	0.56	1.8	.71	55.7	-1.9	0.52	1.2	.83	15R	0	L211
L212	80.8	-5.1	-1.33	3.8	1.49	56.0	-1.6	0.45	1.5	1.03	15T	0	L212
L213	83.2	-2.7	0.70	2.4	.94	59.9	2.2	.60	1.2	.81	15T	0	L213
L217	86.4	.5	.14	1.8	.72	56.9	0.7	0.20	1.1	.77	15R	0	L217
L223	86.3	.4	.11	2.4	.95	58.0	.4	.10	1.3	.86	15R	0	L223
L224	84.7	-1.1	0.30	1.7	.68	58.8	1.2	.31	1.0	.69	15T	0	L224
L225	86.9	1.0	.26	1.7	.68	56.5	-1.2	0.32	1.6	1.08	15T	0	L225
L226B	61.1	-4.8	-1.26	4.7	1.85	60.4	2.8	.75	1.7	1.17	15T	*	L226B
L226C	79.2	-6.7	-1.75	2.4	.94	54.3	-3.4	0.92	1.5	1.01	15T	0	L226C
L228	84.5	-1.3	0.35	1.6	.63	55.5	-2.2	0.59	1.4	.96	15T	0	L228
L230	76.7	0.9	0.23	1.9	.76	51.4	-6.2	-1.68	1.2	.81	15R	0	L230
L232	85.9	1.1	.27	2.8	1.12	60.5	2.9	.78	1.6	1.08	15T	0	L232
L236	87.7	1.8	.47	3.1	1.24	55.6	-2.0	0.56	1.1	.76	15T	0	L236
L237A	83.5	-2.3	0.61	2.2	.87	57.3	0.4	0.10	1.3	.91	15T	0	L237A
L237B	83.7	-2.1	0.56	1.7	.68	55.8	-1.8	0.50	1.3	.90	15T	0	L237B
L238A	83.5	-2.4	0.63	2.9	1.14	54.0	-3.6	0.99	.8	.51	15T	0	L238A
L243	89.3	3.5	.90	2.7	1.07	60.4	2.8	.75	1.2	.80	15T	0	L243
L244	92.9	7.1	1.84	2.1	.81	58.1	.4	.11	1.0	.65	15C	*	L244
L249	88.9	3.0	.78	3.8	1.51	61.8	4.1	1.11	1.4	.95	15T	0	L249
L254	84.7	-1.1	0.30	2.5	1.00	58.0	.4	.10	1.0	.68	15T	0	L254
L255	85.5	0.3	0.09	1.9	.76	55.5	-2.1	0.57	.8	.57	15T	0	L255
L257A	85.5	0.4	0.11	1.6	.63	59.9	2.2	.60	1.9	1.30	15C	0	L257A
L257B	85.6	0.3	0.07	2.0	.80	60.0	2.4	.64	1.7	1.15	15C	0	L257B
L257C	85.2	0.7	0.18	3.1	1.23	60.5	2.9	.78	1.8	1.20	15C	0	L257C
L259	89.1	3.2	.83	2.3	.92	60.1	2.4	.66	1.2	.79	15T	0	L259
L261	82.4	-3.5	0.91	2.8	1.10	56.9	0.7	0.19	1.2	.83	15T	0	L261
L262	86.5	.6	.15	2.0	.78	55.4	-2.2	0.61	1.6	1.11	15T	0	L262

TAPPI STANDARD T414 TS-65. ANY MAKE ELMENDORF WITH DEEP CUTOUT IS STANDARD FOR THIS ANALYSIS

LAB CODE	PRINTING E76 116 GRAMS PER SQUARE METER					WRITING E80 69 GRAMS PER SQUARE METER					TEST D. # 15		
	MEAN	DEV	N.DEV	SDR	R.SDR	MEAN	DEV	N.DEV	SDR	R.SDR	VAR	F	LAB
L264	76.3	-9.6	-2.51	2.8	1.12	59.5	1.8	.49	3.0	2.02	15T	X	L264
L273	87.1	1.2	.31	2.7	1.05	62.7	5.1	1.38	1.1	.75	15T	Ø	L273
L275	89.3	3.5	.90	1.8	.70	56.5	-1.1	-.30	1.6	1.05	15T	Ø	L275
L278	86.4	.5	.14	2.3	.91	51.1	-6.6	-1.79	1.5	1.04	15T	*	L278
L279	83.6	-2.3	-.60	3.0	1.21	57.1	-.6	-.16	1.8	1.24	15T	Ø	L279
L280	87.8	1.9	.50	2.0	.78	56.0	-1.6	-.45	.9	.63	15L	Ø	L280
L281	86.1	.2	.05	2.9	1.14	54.7	-2.9	-.79	1.5	1.04	15T	Ø	L281
L285	89.5	3.6	.94	2.3	.92	60.9	3.3	.89	1.8	1.24	15T	Ø	L285
L288	88.8	2.9	.76	2.0	.78	60.6	2.9	.80	.7	.50	15Q	Ø	L288
L291	81.9	-4.0	-1.05	1.6	.65	54.3	-3.4	-.92	1.1	.75	15A	Ø	L291
L303	87.2	1.3	.34	2.2	.89	57.9	.3	.08	1.5	1.01	15L	Ø	L303
L305	88.9	3.1	.80	3.0	1.19	60.3	2.6	.71	1.3	.87	15T	Ø	L305
L309	86.1	.3	.07	1.9	.76	57.5	-.1	-.03	1.7	1.17	15T	Ø	L309
L312	82.1	-3.7	-.98	3.0	1.18	56.5	-1.1	-.30	1.9	1.30	15T	Ø	L312
L315	90.3	4.4	1.15	4.0	1.60	59.3	1.7	.46	1.5	1.05	15T	Ø	L315
L324	74.9	-10.9	-2.86	4.1	1.64	55.9	-1.8	-.48	1.2	.85	15T	X	L324
L328	84.2	-1.6	-.43	2.6	1.05	52.4	-5.3	-1.43	3.4	2.29	15T	Ø	L328
L331	93.0	7.1	1.86	3.4	1.34	66.9	9.3	2.52	2.9	1.98	15T	*	L331
L336	85.9	-.0	-.00	2.4	.95	56.6	-1.0	-.28	1.6	1.08	15T	Ø	L336
L344	93.7	7.9	2.05	2.4	.94	62.3	4.6	1.25	2.5	1.69	15C	Ø	L344
L345	84.1	-1.7	-.46	4.2	1.68	56.5	-1.1	-.30	1.4	.96	15T	Ø	L345
L352	91.0	5.1	1.34	2.3	.92	61.1	3.5	.94	.9	.63	15C	Ø	L352
L360	68.1	2.2	.57	2.6	1.04	57.2	-.4	-.12	1.7	1.15	15T	Ø	L360
L362	84.4	-1.5	-.39	2.6	1.05	56.0	-1.6	-.45	1.5	1.03	15T	Ø	L362
L366	82.7	-3.1	-.82	2.5	.99	54.1	-3.5	-.95	.7	.50	15T	Ø	L366
L376	90.8	4.9	1.28	2.1	.84	63.1	5.4	1.47	1.9	1.27	15T	Ø	L376
L378	86.3	.4	.10	2.6	1.03	58.4	.8	.20	1.5	1.05	15T	Ø	L378
L382	88.9	3.0	.78	3.3	1.30	60.5	2.9	.78	1.3	.88	15T	Ø	L382
L388	79.9	-6.0	-1.57	3.5	1.38	47.9	-9.8	-2.65	1.0	.67	15T	*	L388
L390	89.3	2.4	.62	2.2	.88	60.5	2.8	.77	1.8	1.20	15T	Ø	L390
L442	95.3	9.4	2.46	2.6	1.05	60.8	3.2	.86	1.4	.95	15R	*	L442
L484	88.4	2.5	.66	1.8	.72	63.3	5.7	1.54	3.5	2.39	15T	Ø	L484
L554	91.2	5.3	1.39	2.7	1.07	60.4	2.8	.75	1.1	.76	15C	Ø	L554
L557	90.0	4.1	1.08	2.3	.92	61.5	3.8	1.04	1.6	1.08	15T	Ø	L557
L558	86.7	.9	.22	1.3	.53	54.8	-2.8	-.77	1.0	.69	15T	Ø	L558
L559	89.5	3.7	.95	1.8	.70	65.7	8.0	2.18	1.3	.88	15T	Ø	L559
L565	83.6	-2.3	-.60	2.5	1.00	53.7	-3.9	-1.06	1.9	1.27	15T	Ø	L565
L566	81.6	-4.3	-1.12	1.7	.68	54.4	-3.2	-.88	1.4	.92	15T	Ø	L566
L575	82.3	-3.6	-.94	3.3	1.30	52.5	-5.2	-1.41	.8	.57	15L	Ø	L575
L576	52.3	6.4	1.67	3.3	1.31	59.5	1.9	.51	1.7	1.14	15T	Ø	L576
L580	86.3	.4	.10	1.5	.61	59.6	2.0	.53	1.1	.72	15T	Ø	L580
L581	88.5	2.7	.69	2.8	1.09	58.7	1.1	.29	1.5	1.05	15Q	Ø	L581
L587	84.1	-1.7	-.46	1.9	.76	57.2	-.4	-.12	1.5	1.00	15T	Ø	L587
L596	79.7	-6.1	-1.61	3.2	1.27	52.3	-5.4	-1.46	2.4	1.61	15T	Ø	L596
L597	81.0	-4.9	-1.28	2.0	.79	54.4	-3.2	-.88	2.3	1.56	15T	Ø	L597
L599	88.9	3.1	.80	2.7	1.07	59.4	1.8	.48	1.4	.95	15T	Ø	L599
L600	86.1	.3	.07	2.7	1.08	61.2	3.6	.96	1.4	.93	15T	Ø	L600
L604	75.2	-10.7	-2.79	3.1	1.23	47.5	-10.2	-2.76	2.6	1.74	15T	*	L604
L606	91.7	5.8	1.51	3.2	1.28	61.3	3.7	1.00	1.4	.95	15T	Ø	L606
L618	19.5	-66.4	-17.35	.9	.36	13.9	-43.8	-11.88	.5	.35	15T	#	L618
L622	82.0	-3.9	-1.01	3.0	1.19	50.8	-6.8	-1.86	1.0	.69	15T	Ø	L622
L651	90.3	4.4	1.15	2.3	.89	59.6	2.0	.53	.8	.56	15T	Ø	L651
L670	80.9	-5.0	-1.31	3.3	1.31	55.9	-1.7	-.46	3.1	2.08	15T	Ø	L670
L676	84.4	-1.5	-.39	2.6	1.05	58.9	1.2	.33	2.1	1.40	15T	Ø	L676

GR. MEAN = 85.9 GRAMS GRAND MEAN = 57.6 GRAMS TEST DETERMINATIONS = 15
SD MEANS = 3.8 GRAMS SD OF MEANS = 3.7 GRAMS 115 LABS IN GRAND MEANS
AVERAGE SDR = 2.5 GRAMS AVERAGE SDR = 1.5 GRAMS
GR. MEAN = 842.2 MILLINEWTON GRAND MEAN = 565.3 MILLINEWTON

L242	88.9	3.1	.80	3.0	1.19	58.9	1.3	.35	1.4	.94	15U	*	L242
L251	85.5	-.4	-.11	1.5	.60	56.4	-1.2	-.34	1.1	.76	15K	*	L251
L299	86.5	.7	.17	3.6	1.42	58.4	.8	.20	1.7	1.17	15V	*	L299
L311	87.5	1.6	.41	1.3	.52	58.3	.6	.17	1.2	.83	15V	*	L311
L396M	86.6	.7	.19	3.7	1.45	57.8	.2	.04	1.5	1.03	15V	*	L396M
L610	84.1	-1.7	-.46	2.4	.95	55.1	-2.6	-.70	1.3	.87	15E	*	L610

TOTAL NUMBER OF LABORATORIES REPORTING = 125

Best values: E76 86 + 6 grams
E80 58 + 5 grams

The following laboratories were omitted from the grand means because of extreme test results: 145

Data from the following laboratories appear to be off by a multiplicative factor: 618

Data from the following laboratories appeared to be off by a multiplicative factor: 299,

311, 396M. Code 15V was assigned temporarily to put in a factor of 2.

Please see the diagram on the inside of the back cover of this report which shows how to distinguish between an Elmendorf tear tester with DEEP CUTOUT and an older model tester with NO CUTOUT.

ANALYSIS T15-1 TABLE 2
TEARING STRENGTH, GRAMS

TAPPI STANDARD T414 TS=65, ANY MAKE ELMENDORF WITH DEEP CUTOUT IS STANDARD FOR THIS ANALYSIS


LAB CODE	F	MHANS		COORDINATES		AVG E.SDR	VAR	PROPERTY	TEST	INSTRUMENT	CONDITIONS
		E76	E80	MAJOR	MINOR						
L618	#	19.5	13.9	-78.3	14.0	.36	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L207	*	74.4	47.1	-15.5	.3	1.16	15R	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF, DIGITAL READOUT
L324	X	74.9	55.9	-9.2	6.2	1.24	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L604	*	75.2	47.5	-14.8	=0	1.48	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L264	X	76.3	59.5	=5.7	7.9	1.57	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L230	0	76.7	51.4	-10.9	1.8	.78	15R	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF, DIGITAL READOUT
L182A	0	79.1	52.3	-8.6	.7	1.21	15A	TEARING	STRENGTH	STANDARD	APPITA
L226C	0	79.2	54.3	-7.2	2.2	.97	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L191	0	79.4	51.0	-9.3	=.4	1.32	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L596	0	79.7	52.3	-8.2	.3	1.44	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L388	*	79.9	47.9	-11.1	=2.9	1.03	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L122	0	80.6	54.1	-6.2	1.1	.80	15C	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (W.AIR CLAMP)
L212	0	80.8	56.0	-4.8	2.3	1.26	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L670	0	80.9	55.9	-4.8	2.2	1.69	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L597	0	81.0	54.4	-5.8	1.0	1.17	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L226B	0	81.1	60.4	-1.6	5.3	1.51	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L566	0	81.6	54.4	-5.3	.6	.80	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L291	0	81.9	54.3	-5.2	.3	.70	15A	TEARING	STRENGTH	STANDARD	APPITA
L622	0	82.0	50.8	-7.5	=2.3	.94	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L145	#	82.1	72.7	7.6	13.5	1.16	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L131	0	82.1	54.9	-4.6	.6	1.61	15A	TEARING	STRENGTH	STANDARD	APPITA
L12	0	82.1	56.5	-3.5	1.8	1.24	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L13	0	82.1	55.1	-4.4	.8	.61	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L158	0	82.3	58.4	-2.1	3.0	1.72	15R	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF, DIGITAL READOUT
L575	0	82.3	52.5	-6.2	-1.3	.94	15L	TEARING	STRENGTH	STANDARD	LORENTZ-WETTRES
L261	0	82.4	56.9	-3.0	1.9	.66	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L366	0	82.7	54.1	-4.7	=.4	.75	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L121	0	82.9	57.9	-2.0	2.2	1.00	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L213	0	83.2	59.9	-4	3.5	.87	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L238A	0	83.5	54.0	-4.3	-1.0	.83	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L170	0	83.5	54.4	-3.9	=.7	.46	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L185	0	83.5	58.1	-1.4	2.0	.97	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L237A	0	83.5	57.3	-2.0	1.3	.89	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L555	0	83.6	53.7	-4.3	-1.3	1.14	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L279	0	83.6	57.1	-2.1	1.2	1.22	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L237B	0	83.7	55.8	-2.8	.1	.79	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L211	0	83.7	55.7	-2.9	.1	.77	15R	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF, DIGITAL READOUT
L610	*	84.1	55.1	-3.0	=.7	.91	15H	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF, AMBIENT COND.
L587	0	84.1	57.2	-1.6	.9	.88	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L345	0	84.1	56.5	-2.0	.4	1.32	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L328	0	84.2	52.4	-4.8	=2.7	1.67	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L676	0	84.4	58.9	=.2	1.9	1.22	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L362	0	84.4	56.0	-2.2	=.2	1.04	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L100	0	84.5	53.9	-3.6	-1.8	.85	15M	TEARING	STRENGTH	STANDARD	T. M. MIRFIELD (APPITA-ELMENDORF)
L228	0	84.5	55.5	-2.5	=.7	.79	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L105	0	84.6	55.1	-2.7	=.9	1.01	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L190C	0	84.6	58.3	=.5	1.3	1.06	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L224	0	84.7	58.8	=.0	1.6	.68	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L254	0	84.7	58.0	=.6	1.0	.84	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L148	*	84.8	65.1	4.3	6.1	1.18	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L173B	0	84.8	61.6	1.9	3.6	.71	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L163	0	84.9	57.5	=.9	.6	1.16	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L128	0	84.9	56.0	-1.8	=.5	.87	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L257C	0	85.2	60.5	1.5	2.6	1.21	15C	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (W.AIR CLAMP)
L167	0	85.3	60.7	1.7	2.6	.52	15C	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (W.AIR CLAMP)
L251	*	85.5	56.4	-1.2	=.6	.68	15K	TEARING	STRENGTH	STANDARD	LORENTZ-WETTRES, 20 C, 65% RH
L257A	0	85.5	59.9	1.2	1.9	.97	15C	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (W.AIR CLAMP)
L255	0	85.5	55.5	-1.7	-1.3	.66	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L257B	0	85.6	60.0	1.4	1.9	.98	15C	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (W.AIR CLAMP)
L336	0	85.9	56.6	=.7	=.7	1.01	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L141	0	85.9	57.6	.0	=.1	.89	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L190R	0	86.1	56.9	=.4	=.6	1.01	15C	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (W.AIR CLAMP)
L283	0	86.1	54.7	-1.9	=2.2	1.09	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L60C	0	86.1	61.2	2.6	2.4	1.01	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)
L309	0	86.1	57.5	.1	=.3	.97	15T	TEARING	STRENGTH	STANDARD	THWING-ELMENDORF (SCALE T0 100)

TAPPI STANDARD T414 TS-65. ANY MAKE ELMENDORF WITH DEEP CUTOUT IS STANDARD FOR THIS ANALYSIS

LAB CODE	F	MEANS		COORDINATES		AVG R. SDR	VAR	PROPERTY==TEST	INSTRUMENT==CONDITIONS
		E76	E80	MAJOR	MINOR				
L189	Ø	86.2	56.2	0.8	-1.3	.92	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L580	Ø	86.3	59.6	1.6	1.2	.66	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L378	Ø	86.3	58.4	.8	.3	1.04	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L223	Ø	86.3	58.0	.6	-0.0	.91	15R	TEARING STRENGTH,	STANDARD, TEWING=ELMENDORF, DIGITAL READOUT
L134	Ø	86.3	56.7	-0.3	-1.0	.74	15C	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (W.AIR CLAMP)
L217	Ø	86.4	56.9	-0.1	-0.9	.75	15R	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF, DIGITAL READOUT
L278	*	86.4	51.1	-0.2	-0.1	.98	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L262	Ø	86.5	55.4	-1.1	-2.0	.94	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L299	*	86.5	58.4	1.0	.1	1.30	15V	TEARING STRENGTH,	STANDARD, TEWING=ELMENDORF (SCALE TØ 100)X2
L396M	*	86.6	57.8	.6	-0.4	1.24	15V	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)X2
L558	Ø	86.7	54.8	-1.3	-2.6	.61	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L225	Ø	86.9	56.5	-0.1	-1.5	.88	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L232	Ø	86.9	60.5	2.7	1.4	1.10	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L162	Ø	87.1	57.6	.8	-0.8	.87	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L273	Ø	87.1	62.7	4.4	2.9	.90	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L183	Ø	87.1	56.1	-0.2	-1.9	.78	15T	TEARING STRENGTH,	STANDARD, TEWING=ELMENDORF (SCALE TØ 100)
L303	Ø	87.2	57.9	1.2	-0.7	.95	15L	TEARING STRENGTH,	STANDARD, LORENTZ=WETTRES
L311	*	87.5	58.3	1.6	-0.6	.67	15V	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)X2
L143	Ø	87.5	57.7	1.2	-1.1	1.74	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L124	Ø	87.6	60.3	3.0	.7	.90	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L236	Ø	87.7	55.6	-0.1	-2.7	1.00	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L159	Ø	87.7	58.0	1.6	-1.0	1.50	15L	TEARING STRENGTH,	STANDARD, LORENTZ=WETTRES
L280	Ø	87.8	56.0	.3	-2.5	.71	15L	TEARING STRENGTH,	STANDARD, LORENTZ=WETTRES
L176	Ø	87.9	58.0	1.7	-1.1	1.03	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L150	Ø	87.9	57.9	1.7	-1.2	.91	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L360	Ø	88.1	57.2	1.3	-1.8	1.10	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L126	Ø	88.3	59.1	2.7	-0.6	1.20	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L390	Ø	88.3	60.5	3.7	.4	1.04	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L484	Ø	88.4	63.3	5.7	2.4	1.55	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L107	*	88.5	65.6	7.4	3.9	4.22	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L581	Ø	88.5	58.7	2.7	-1.1	1.07	15Q	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF, AIR CLAMP, DIGITL
L166	Ø	88.7	58.2	2.4	-1.5	.96	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L288	Ø	88.8	60.6	4.1	.1	.64	15Q	TEARING STRENGTH,	STANDARD, TEWING=ELMENDORF, AIR CLAMP, DIGITL
L249	Ø	88.9	61.8	5.0	.9	1.23	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L382	Ø	88.9	60.5	4.2	.0	1.09	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L206	Ø	88.9	60.3	4.0	-0.2	.99	15R	TEARING STRENGTH,	STANDARD, TEWING=ELMENDORF, DIGITAL READOUT
L242	*	88.9	58.9	3.1	-1.2	1.07	15U	TEARING STRENGTH,	STANDARD, AUSTRALIAN OPT. CØ.
L305	Ø	88.9	60.3	4.0	-0.2	1.03	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L599	Ø	88.9	59.4	3.4	-0.8	1.01	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L259	Ø	89.1	60.1	4.0	-0.4	.85	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L243	Ø	89.3	60.4	4.4	-0.4	.94	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L275	Ø	89.3	56.5	1.7	-3.2	.88	15T	TEARING STRENGTH,	STANDARD, TEWING=ELMENDORF (SCALE TØ 100)
L195	Ø	89.5	56.1	1.6	-3.6	.91	15C	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (W.AIR CLAMP)
L285	Ø	89.5	60.9	4.9	-0.1	1.08	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L559	Ø	89.5	65.7	8.2	3.3	.79	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L557	Ø	90.0	61.5	5.6	-0.1	1.00	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L651	Ø	90.3	59.6	4.5	-1.6	.73	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L315	Ø	90.3	59.3	4.3	-1.8	1.33	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L182T	Ø	90.3	60.1	4.9	-1.2	1.07	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L376	Ø	90.8	63.1	7.3	.5	1.05	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L352	Ø	91.0	61.1	6.1	-1.0	.77	15C	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (W.AIR CLAMP)
L554	Ø	91.2	60.4	5.8	-1.7	.92	15C	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (W.AIR CLAMP)
L606	Ø	91.7	61.3	6.7	-1.3	1.11	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L139	Ø	92.1	63.8	8.8	.2	.90	15T	TEARING STRENGTH,	STANDARD, TEWING=ELMENDORF (SCALE TØ 100)
L576	Ø	92.3	59.5	5.9	-3.0	1.23	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L244	*	92.9	58.1	5.4	-0.5	.73	15C	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (W.AIR CLAMP)
L331	*	93.0	66.9	11.6	1.8	1.66	15T	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (SCALE TØ 100)
L151	Ø	93.7	66.0	11.4	.7	1.08	15C	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (W.AIR CLAMP)
L344	Ø	93.7	62.3	8.9	-2.1	1.32	15C	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF (W.AIR CLAMP)
L442	*	95.3	60.8	9.0	-0.2	1.00	15R	TEARING STRENGTH,	STANDARD, THWING=ELMENDORF, DIGITAL READOUT
GMEANS:		85.9	57.6			1.00			
		95% ELLIPSE:	12.3	4.8				WITH GAMMA = 43 DEGREES	


TEARING STRENGTH, DEEP CUTOUT

SAMPLE E76 = 86. GRAMS SAMPLE E80 = 58. GRAMS
 SAMPLE E76 = 842 MILLINEWTON SAMPLE E80 = 565 MILLINEWTON

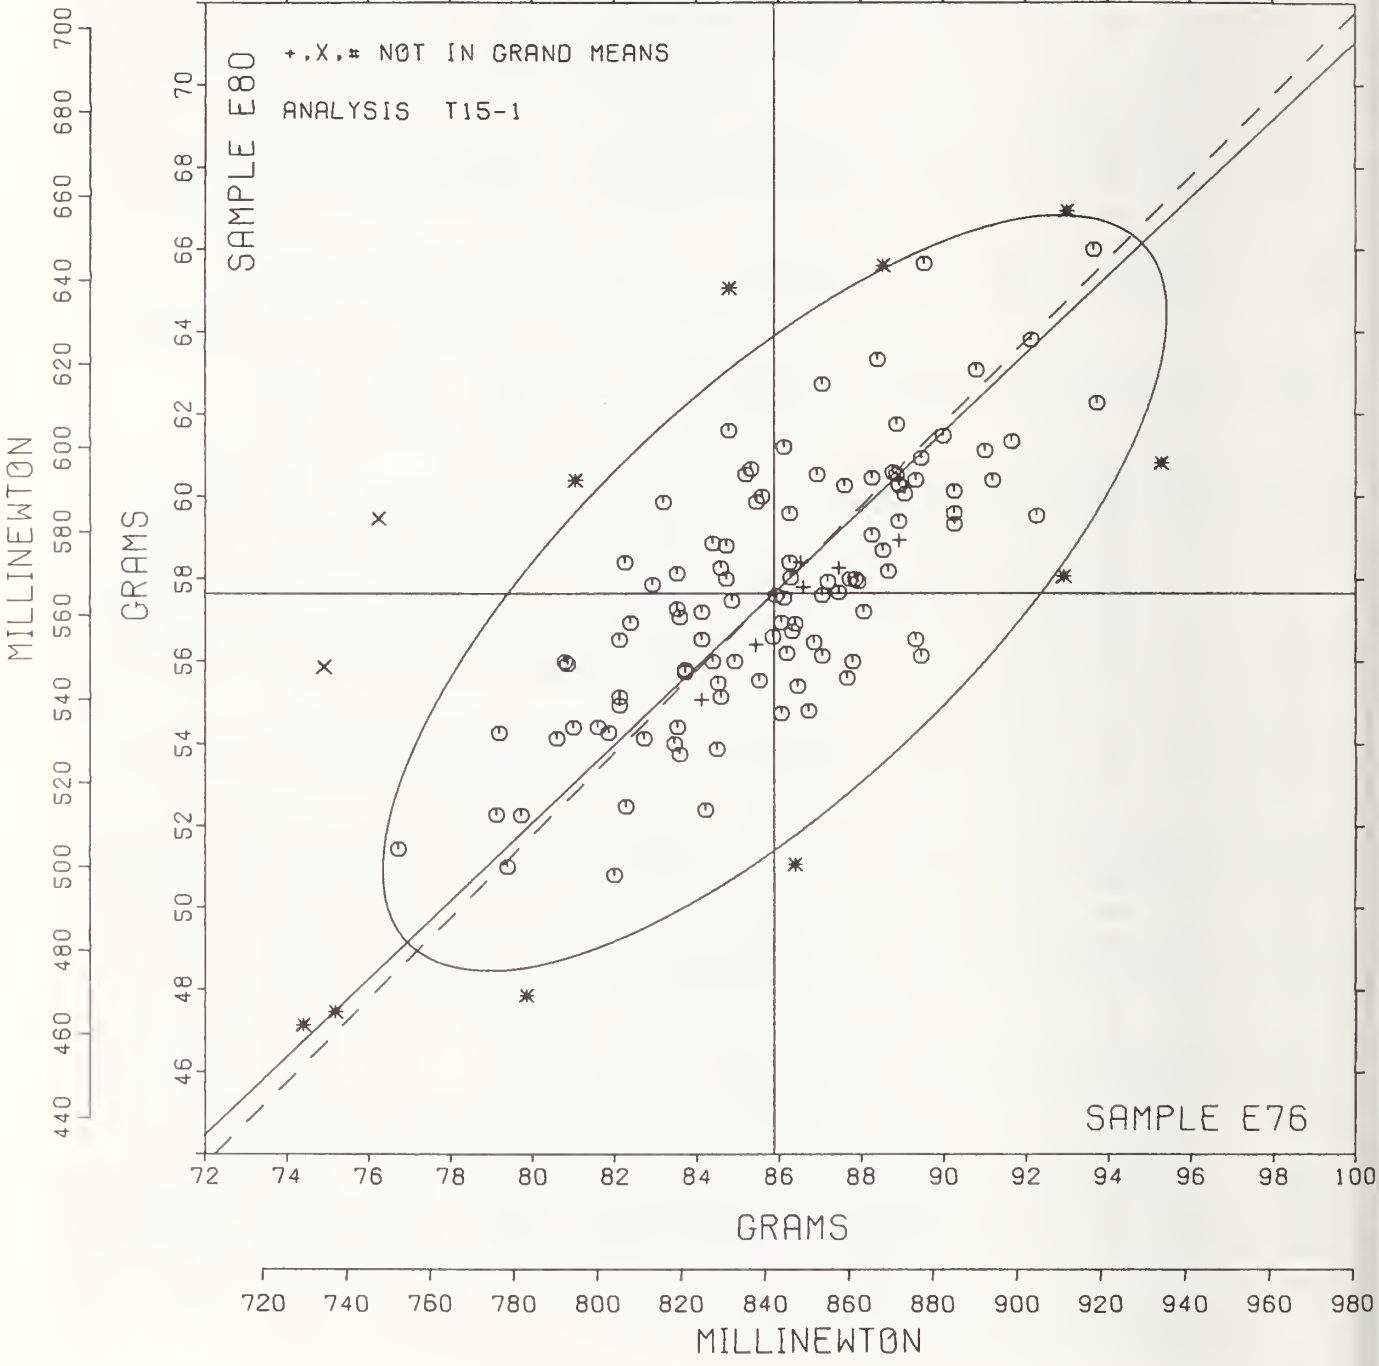

TEARING STRENGTH, NO CUTOUT

SAMPLE J41 = 67. GRAMS SAMPLE K19 = 151. GRAMS
 SAMPLE J41 = 659 MILLINEWTON SAMPLE K19 = 1486 MILLINEWTON

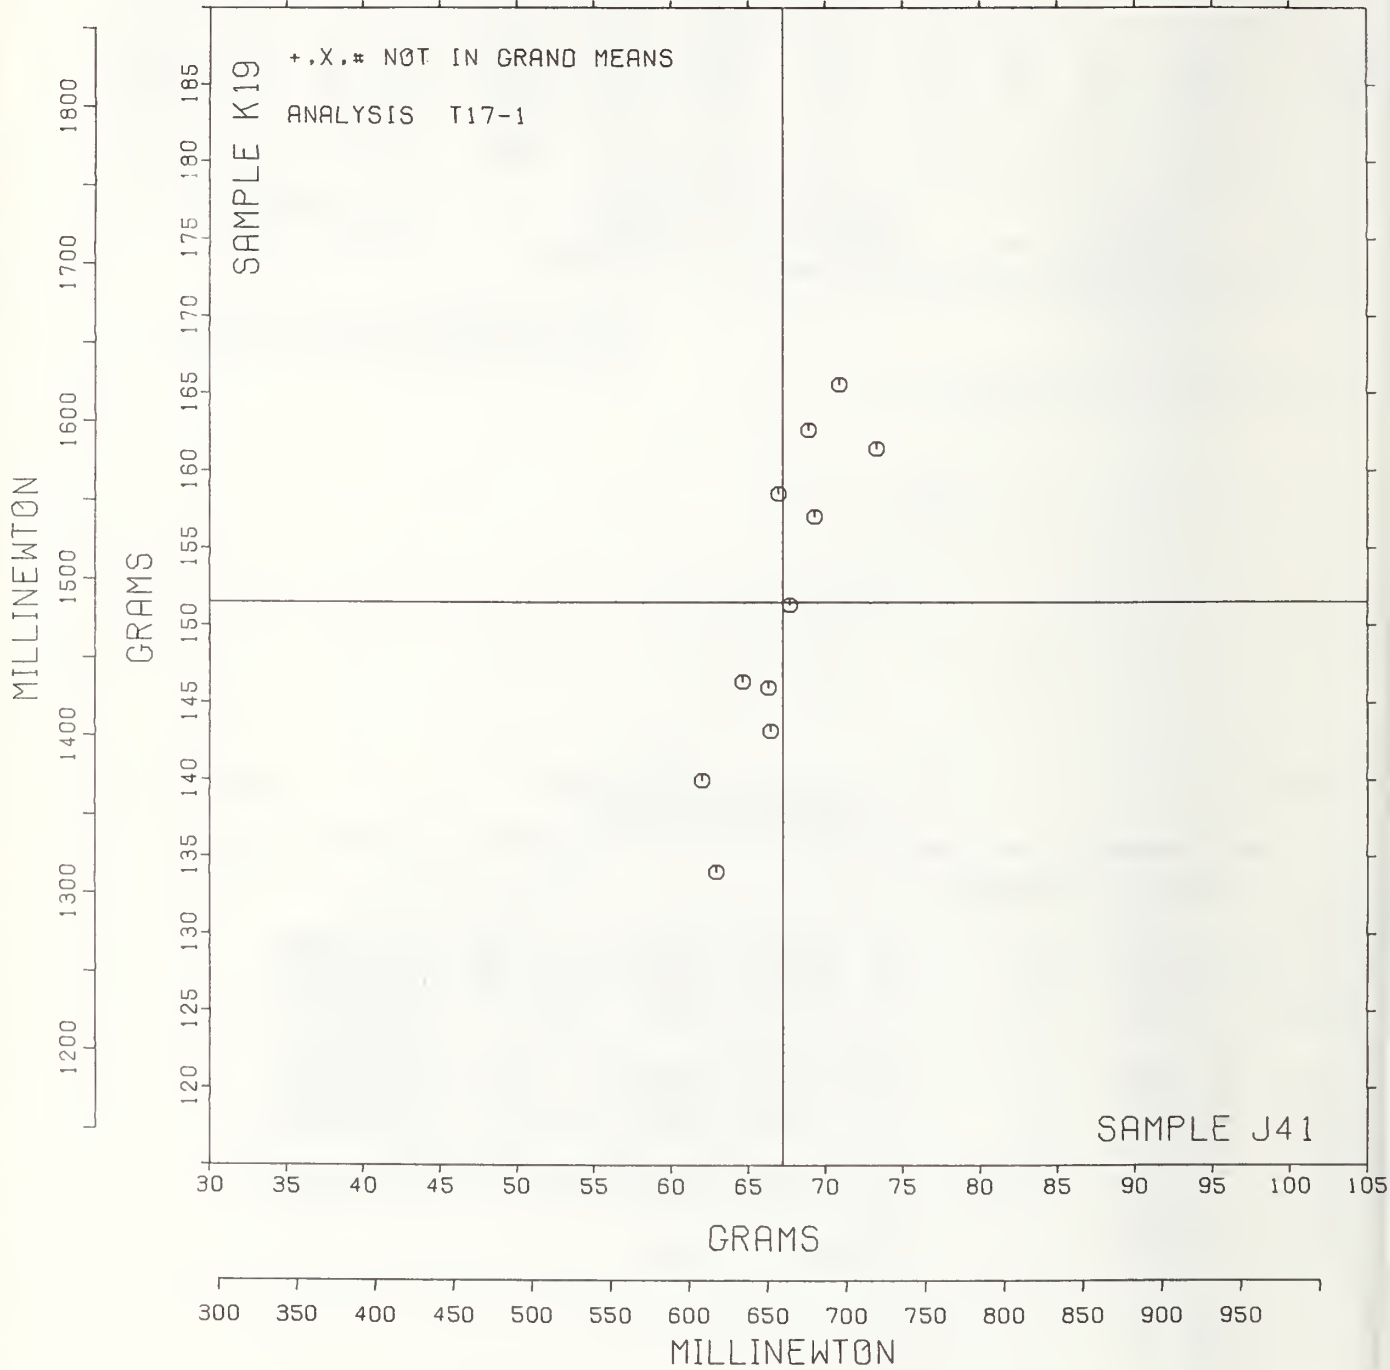

TENSILE BREAKING STRENGTH, KILOWEIGHTS PER METER - PACKAGING PAPER
TAPPI STANDARDS T404 CS-76 AND T494 CS-70, TENSILE BREAKING STRENGTH, PENDULUM AND CRE TYPES

LAB CODE	SAMPLE J15 149 GRAMS PER SQUARE METER					SAMPLE K31 105 GRAMS PER SQUARE METER					TEST D. = 20		
	MEAN	DEV	N.DEV	SDR	R. SDR	MEAN	DEV	N.DEV	SDR	R. SDR	VAR	F	LAB
L100	8.74	.16	.48	.25	.79	8.92	.34	1.13	.38	.83	19E	0	L100
L107	8.97	.39	1.19	.28	.87	8.92	.33	1.10	.36	.80	19A	0	L107
L122	8.69	.11	.33	.32	1.00	8.69	.11	.37	.43	.94	19A	0	L122
L126	8.48	-.10	-.30	.25	.80	8.65	.06	.21	.47	1.04	19A	0	L126
L151	8.76	.18	.56	.37	1.17	8.47	-.11	-.37	.40	.88	19A	0	L151
L167	9.63	1.05	3.17	.33	1.06	9.93	1.35	4.45	.49	1.09	19G	#	L167
L182I	8.12	-.46	-1.39	.27	.85	8.35	-.23	-.76	.41	.92	19D	0	L182I
L182L	8.54	-.04	-.13	.33	1.05	8.56	-.02	-.08	.46	1.01	19T	0	L182L
L207	8.59	.01	.03	.33	1.05	8.50	-.08	-.26	.49	1.09	19A	0	L207
L217A	8.45	-.13	-.39	.24	.77	8.85	.27	.88	.34	.76	19A	0	L217A
L217P	8.51	-.07	-.20	.45	1.42	8.89	.31	1.01	.37	.81	19P	0	L217P
L224	8.40	-.18	-.55	.34	1.07	9.00	.42	1.37	.42	.93	19A	*	L224
L225	8.65	.07	.20	.21	.67	8.55	-.03	-.09	.56	1.24	19P	0	L225
L234L	8.43	-.15	-.44	.39	1.22	8.66	.08	.27	.43	.94	19P	0	L234L
L237A	8.30	-.28	-.85	.44	1.41	7.09	-1.49	-4.91	.60	1.33	19Q	#	L237A
L237B	5.32	.74	2.22	.36	1.14	9.02	.44	1.43	.63	1.40	19A	0	L237B
L238A	8.82	.24	.72	.38	1.20	8.55	-.04	-.12	.43	.94	15T	0	L238A
L243	8.37	-.21	-.63	.27	.86	8.72	.14	.45	.33	.72	19A	0	L243
L257A	8.56	.01	.03	.34	1.08	8.48	-.10	-.34	.36	.80	19P	0	L257A
L257C	8.53	-.05	-.16	.24	.76	8.55	-.03	-.11	.41	.91	19P	0	L257C
L264A	8.79	.21	.63	.41	1.29	8.69	.11	.35	.51	1.12	19A	0	L264A
L264P	9.18	.60	1.80	.28	.89	9.10	.51	1.69	.42	.93	19P	0	L264P
L265	8.11	-.47	-1.41	.22	.69	8.62	.04	.12	.42	.93	19A	0	L265
L267	8.52	-.06	-.17	.33	1.05	8.92	.34	1.11	.42	.93	19A	0	L267
L273	6.68	.11	.32	.37	1.16	8.75	.17	.57	.49	1.07	19P	0	L273
L280	7.75	-.83	-2.51	.49	1.56	7.87	-.71	-2.35	.56	1.24	19G	*	L280
L281	8.77	.19	.57	.35	1.09	8.91	.33	1.08	.41	.90	19G	0	L281
L305	8.77	.19	.57	.23	.74	8.35	-.24	-.78	.35	.78	19V	0	L305
L312	8.80	.22	.66	.26	.83	8.66	.08	.27	.34	.74	19D	0	L312
L318	8.11	-.47	-1.42	.25	.81	8.04	-.54	-1.79	.39	.87	19G	0	L318
L324	8.57	-.01	-.02	.29	.92	8.66	.08	.26	.42	.92	19A	0	L324
L336	5.03	.45	1.36	.38	1.20	8.63	.05	.17	.67	1.47	19G	0	L336
L356	9.03	.45	1.35	.26	.81	8.74	.16	.51	.51	1.12	19P	0	L356
L366	8.69	-.49	-1.46	.50	1.58	8.35	-.23	-.76	.39	.87	19P	0	L366
L565	8.66	.08	.24	.19	.59	8.49	-.09	-.30	.31	.68	19T	0	L565
L568	8.22	-.36	-1.08	.42	1.34	7.94	-.65	-2.13	.29	.63	19P	0	L568
L575	8.54	-.04	-.13	.23	.74	8.50	-.08	-.27	.36	.80	19G	0	L575
L576	8.44	-.14	-.43	.24	.78	8.32	-.26	-.87	.55	1.22	19A	0	L576
L580	8.94	.36	1.09	.31	.98	8.60	.02	.06	.42	.93	19G	0	L580
L581	8.76	.18	.56	.29	.91	8.79	.21	.68	.44	.97	19A	0	L581
L582	7.91	-.67	-2.03	.35	1.12	7.95	-.63	-2.08	.57	1.25	19A	0	L582
L604	8.45	-.13	-.40	.43	1.36	8.35	-.23	-.76	.53	1.17	19P	0	L604
L606	8.16	-.42	-1.28	.28	.90	8.27	-.31	-1.03	.51	1.13	19P	0	L606
L610	8.54	-.04	-.13	.34	1.09	8.38	-.20	-.67	.43	.96	19A	0	L610
L622	8.90	.33	.98	.32	1.01	8.76	.18	.59	.56	1.24	190	0	L622
L650	9.06	.48	1.44	.46	1.44	9.13	.54	1.79	.56	1.23	19G	0	L650
L676	8.35	-.23	-.68	.31	.99	8.11	-.47	-1.56	.94	2.08	19A	0	L676

GR. MEAN = 8.58 KILOWEIGHTS/M GRAND MEAN = 8.58 KILOWEIGHTS/M TEST DETERMINATIONS = 20
SD MEANS = .33 KILOWEIGHTS/M SD OF MEANS = .30 KILOWEIGHTS/M 45 LABS IN GRAND MEANS
AVERAGE SDR = .32 KILOWEIGHTS/M AVERAGE SDR = .45 KILOWEIGHTS/M
GR. MEAN = 49.00 LB/INCH GRAND MEAN = 49.01 LB/INCH

L251 7.63 -.95 -2.85 .45 1.43 7.66 -.92 -3.04 .70 1.56 19I * L251
TOTAL NUMBER OF LABORATORIES REPORTING = 48

Best values: J15 8.6 ± 0.5 kilonewton per meter
K31 8.6 ± 0.5 kilonewton per meter


The following laboratories were omitted from the grand means because of extreme test results: 167, 237A

TENSILE BREAKING STRENGTH, KILOWEIGHTS PER METER - PACKAGING PAPER
TAPPI STANDARDS T404 GS-76 AND T494 GS-70, TENSILE BREAKING STRENGTH, PENDULUM AND CRE TYPES

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST	INSTRUMENT---CONDITIONS
		J45	K31	MAJOR	MINOR	R.SDR	VAR		
L251	*	7.63	7.66	-1.32	-0.07	1.49	19I	TENSILE STRENGTH,	PACKAGING PAPER, CRE, 20C, 65% RH
L280	*	7.75	7.87	-1.10	.02	1.40	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L582	Ø	7.91	7.95	-.92	-0.03	1.18	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L366	Ø	8.09	8.35	-.52	.15	1.22	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L318	Ø	8.11	8.04	-.71	-.10	.84	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L265	Ø	8.11	8.62	-.33	.34	.81	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L182I	Ø	8.12	8.35	-.50	.13	.89	19D	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L606	Ø	8.16	8.27	-.52	.05	1.01	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L568	Ø	8.22	7.94	-.70	-.25	.99	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L237A	#	8.30	7.09	-1.20	-.93	1.37	19Q	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L676	Ø	8.35	8.11	-.48	-.21	1.54	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L243	Ø	8.37	8.72	-.07	.24	.79	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L224	*	8.40	9.00	.14	.43	1.00	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L234L	Ø	8.43	8.66	-.06	.16	1.08	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L576	Ø	8.44	8.32	-.28	-.10	1.00	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L604	Ø	8.45	8.35	-.25	-.09	1.27	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L217A	Ø	8.45	8.85	.08	.29	.76	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L126	Ø	8.48	8.65	-.03	.11	.92	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L217P	Ø	8.51	8.89	.15	.27	1.12	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L267	Ø	8.52	8.92	.18	.29	.99	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L257C	Ø	8.53	8.55	-.06	.01	.83	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L182L	Ø	8.54	8.56	-.05	.01	1.03	19T	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L610	Ø	8.54	8.38	-.17	-.12	1.03	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L575	Ø	8.54	8.50	-.09	-.03	.77	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L324	Ø	8.57	8.66	.05	.06	.92	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L207	Ø	8.59	8.50	-.05	-.07	1.07	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L257A	Ø	8.59	8.48	-.06	-.08	.94	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L225	Ø	8.65	8.55	.03	-.07	.95	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L565	Ø	8.66	8.49	-.00	-.12	.64	19T	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L273	Ø	8.68	8.75	.19	.06	1.12	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L122	Ø	8.69	8.69	.16	.01	.97	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L100	Ø	8.74	8.92	.35	.15	.81	19E	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L151	Ø	8.76	8.47	.06	-.21	1.02	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L581	Ø	8.76	8.79	.28	.03	.94	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L305	Ø	8.77	8.35	-.02	-.30	.76	19V	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L281	Ø	8.77	8.91	.36	.12	1.00	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L264A	Ø	8.79	8.69	.23	-.05	1.21	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L312	Ø	8.80	8.66	.22	-.08	.79	19D	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L238A	Ø	8.82	8.55	.16	-.19	1.07	19T	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L622	Ø	8.90	8.76	.36	-.08	1.12	19G	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L580	Ø	8.94	8.60	.28	-.23	.95	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L107	Ø	8.97	8.92	.52	-.01	.84	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L355	Ø	9.03	8.74	.44	-.18	.96	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L336	Ø	9.03	8.63	.37	-.26	1.34	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L650	Ø	9.06	9.13	.72	.09	1.34	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L264P	Ø	9.18	9.10	.79	-.01	.91	19P	TENSILE STRENGTH,	PACKAGING PAPER, PENDULUM TESTER
L2378	Ø	9.32	9.02	.84	-.16	1.27	19A	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
L167	#	9.63	9.93	1.68	.32	1.08	19G	TENSILE STRENGTH,	PACKAGING PAPER, LOAD CELL (CRE)
GMEANS:		8.58	8.58			1.00			
95% ELLIPSE:				1.07	.44			WITH GAMMA = 41 DEGREES	

TENSILE STRENGTH, PACKAGING PAPERS

SAMPLE J15 = 8.58 KILONEWTON/M SAMPLE K31 = 8.58 KILONEWTON/M
 SAMPLE J15 = 49.0 LB/INCH SAMPLE K31 = 49.0 LB/INCH

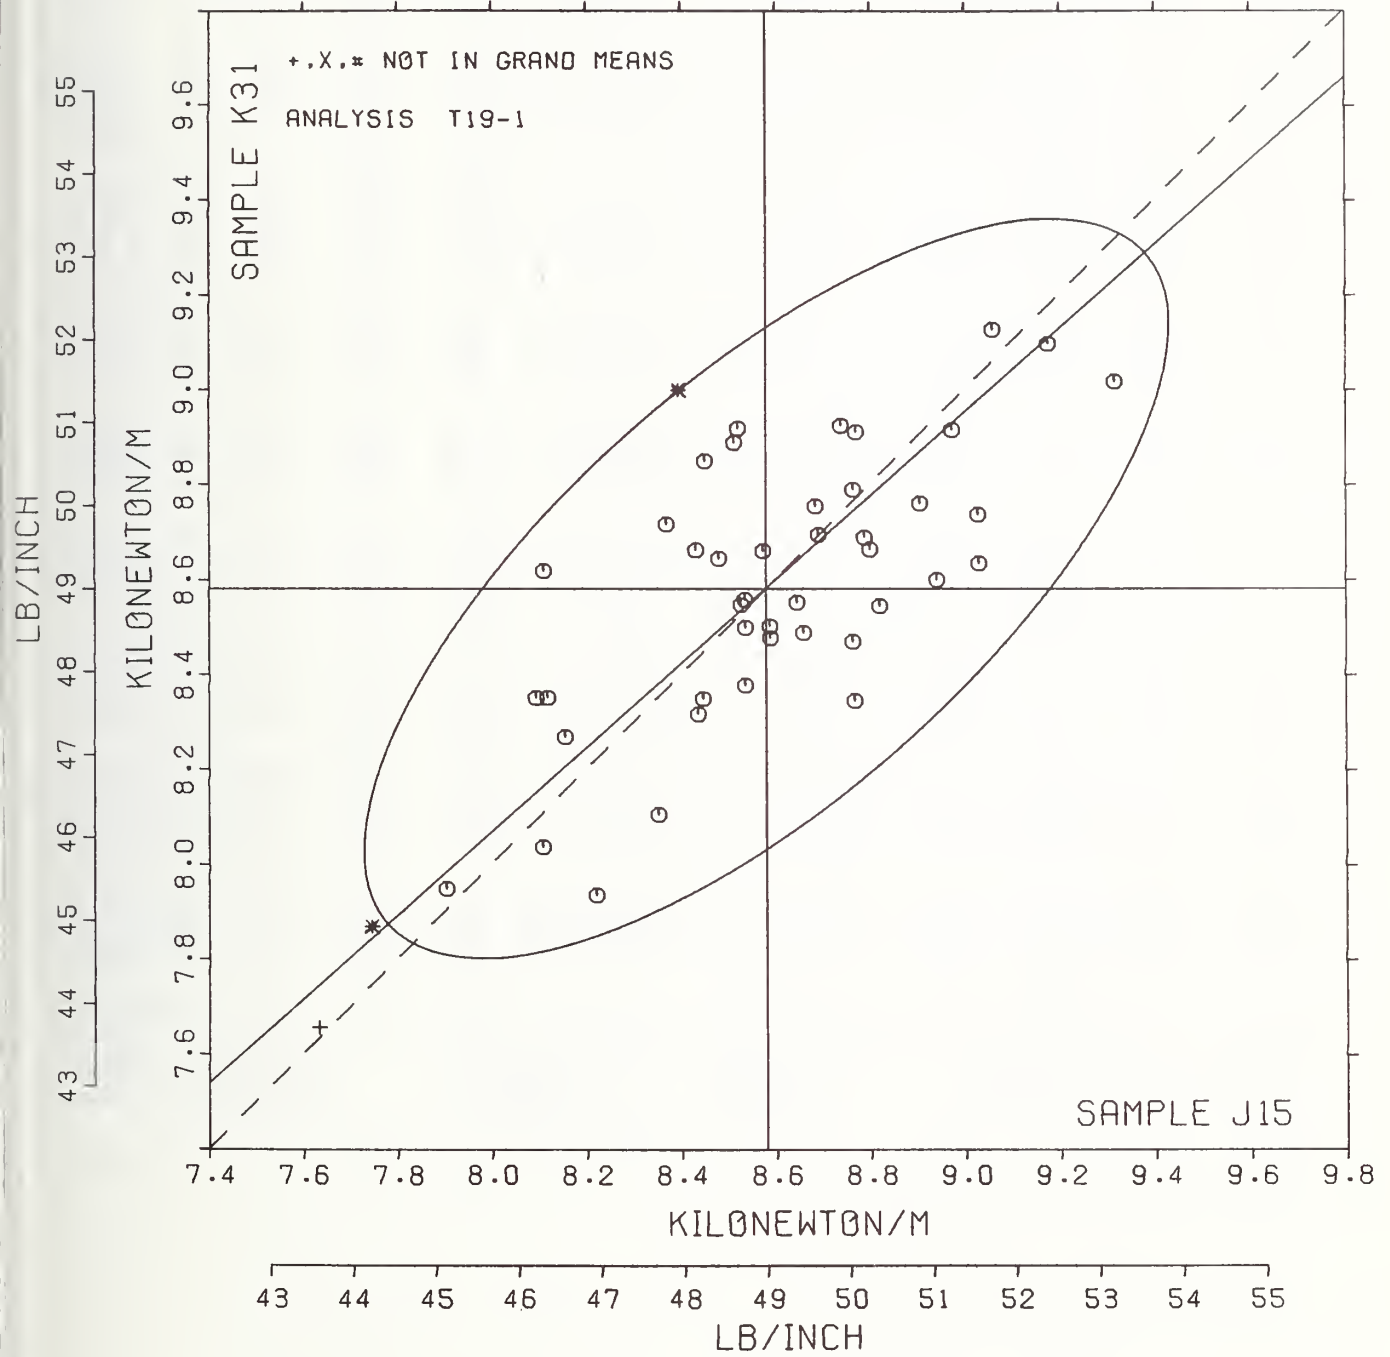

TENSILE BREAKING STRENGTH, KILONEWTONS PER METER
TAPPI STANDARD T494 G9-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	SAMPLE J04 73 GRAMS PER SQUARE METER					SAMPLE J08 85 GRAMS PER SQUARE METER					TEST D. = 20		
	MEAN	DEV	N. DEV	SDR	R. SDR	MEAN	DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L100	3.62	0.05	0.28	.17	.99	6.22	.14	.46	.19	.51	20E	0	L100
L105	3.55	0.12	0.67	.20	1.16	6.46	.38	1.27	.55	1.47	20A	*	L105
L122	3.89	0.22	1.23	.15	.86	6.27	.18	.63	.40	1.06	20A	0	L122
L124C	3.52	0.15	0.86	.21	1.24	5.82	0.27	0.92	.39	1.05	20A	0	L124C
L125	3.86	.19	1.05	.19	1.15	6.17	.08	.29	.65	1.74	20C	0	L125
L131	3.97	.30	1.66	.11	.64	6.54	.46	1.54	.33	.88	20E	0	L131
L141T	3.78	.11	.61	.11	.68	6.16	.07	.23	.38	1.01	20A	0	L141T
L143	3.36	0.32	1.77	.17	1.00	5.41	0.67	2.28	.31	.83	20E	0	L143
L148	3.74	.07	.40	.17	1.01	5.99	0.10	0.35	.24	.64	20A	0	L148
L155	3.79	.12	.65	.12	.69	6.22	.13	.45	.42	1.11	20A	0	L155
L163	3.81	.14	.76	.19	1.11	6.41	.32	1.08	.16	.42	20D	0	L163
L167	4.02	.35	1.94	.22	1.29	6.67	.58	1.97	.50	1.32	20G	0	L167
L176	3.39	0.29	1.60	.19	1.13	5.64	0.45	1.53	.34	.91	20E	0	L176
L185	3.73	.06	.32	.22	1.29	6.30	.21	.70	.31	.83	20C	0	L185
L190R	3.64	0.03	0.16	.10	.59	6.02	0.07	0.24	.45	1.20	20A	0	L190R
L223B	3.73	.06	.32	.15	.88	6.25	.16	.55	.28	.74	20A	0	L223B
L226C	3.92	.25	1.38	.27	1.59	6.40	.31	1.04	.67	1.79	20C	0	L226C
L230	3.80	.12	.70	.16	.93	6.45	.36	1.23	.17	.46	20G	0	L230
L243	3.79	.11	.63	.13	.79	6.09	0.00	0.01	.38	1.01	20A	0	L243
L255	3.82	.15	.82	.12	.73	6.33	.25	.83	.20	.53	20A	0	L255
L260	3.57	0.10	0.56	.13	.74	6.06	0.03	0.09	.25	.67	20A	0	L260
L261	3.80	.13	.73	.18	1.04	6.41	.32	1.09	.32	.86	20A	0	L261
L278	3.60	0.07	0.42	.17	1.00	6.15	.07	.22	.29	.77	20A	0	L278
L291	3.19	0.48	2.70	.24	1.41	5.63	0.46	1.56	.54	1.45	20A	*	L291
L309	20.39	16.72	93.55	17.22	101.65	5.64	0.44	1.50	.19	.52	20E	#	L309
L315	3.61	0.06	0.35	.16	.96	6.07	0.02	0.05	.39	1.03	20A	0	L315
L318	3.52	0.15	0.86	.12	.71	5.63	0.45	1.54	.48	1.29	20G	0	L318
L325	3.52	0.16	0.87	.26	1.53	5.90	0.19	0.64	.28	.76	20E	0	L325
L328	3.65	0.02	0.12	.16	.92	5.89	0.20	0.66	.35	.93	20A	0	L328
L331	3.50	0.17	0.97	.20	1.18	5.48	0.61	2.05	.45	1.21	20A	0	L331
L333	3.75	.08	.46	.16	.97	6.13	.04	.13	.40	1.08	20A	0	L333
L344	3.79	.11	.64	.14	.82	6.03	0.06	0.20	.60	1.59	20A	0	L344
L352	3.56	0.11	0.61	.22	1.29	5.84	0.25	0.86	.44	1.17	20A	0	L352
L360	1.26	2.41	13.49	.09	.53	2.13	3.96	13.41	.08	.22	20B	#	L360
L372	.34	3.33	18.62	.03	.17	6.09	.01	.02	.52	1.38	20A	0	L372
L378	3.73	.06	.31	.19	1.12	5.75	0.34	1.14	.56	1.51	20A	0	L378
L390	3.83	.16	.88	.21	1.23	6.37	.28	.94	.35	.93	20A	0	L390
L442	3.51	0.16	0.88	.11	.66	5.91	0.18	0.61	.33	.87	20G	0	L442
L557	3.40	0.27	1.50	.18	1.06	5.93	0.16	0.53	.27	.71	20A	0	L557
L558	.96	2.71	15.18	.18	1.06	1.32	4.77	16.13	.13	.35	20A	#	L558
L559	3.52	0.15	0.83	.11	.67	6.17	.08	.27	.18	.49	20A	0	L559
L563A	3.50	0.18	0.98	.22	1.29	5.79	0.30	1.00	.91	2.42	20A	0	L563A
L575	3.84	.16	.92	.17	1.00	6.46	.37	1.25	.25	.67	20G	0	L575
L587	3.75	.08	.42	.18	1.05	NO DATA REPORTED FOR SAMPLE J08					20A	M	L587
L592	3.66	0.01	0.06	.16	.95	6.10	.01	.05	.29	.79	20A	0	L592
L616	1.17	2.50	14.01	.16	.96	.40	5.69	19.24	.08	.21	20D	#	L616
L618	3.79	.11	.64	.21	1.24	6.10	.01	.03	.46	1.23	20A	0	L618

GR. MEAN = 3.67 KILONEWTON/M GRAND MEAN = 6.09 KILONEWTON/M TEST DETERMINATIONS = 20
SD MEANS = .18 KILONEWTON/M SD OF MEANS = .30 KILONEWTON/M 41 LABS IN GRAND MEANS
AVERAGE SDR = .17 KILONEWTON/M AVERAGE SDR = .37 KILONEWTON/M
GR. MEAN = 12.386 LB/15 MM GRAND MEAN = 20.534 LB/15 MM

L139	3.72	.05	.28	.20	1.17	6.02	0.07	0.23	.30	.81	20H	*	L139
L251	3.20	0.47	2.63	.36	2.12	5.57	0.52	1.74	.41	1.10	20I	*	L251

TOTAL NUMBER OF LABORATORIES REPORTING = 49

Best values: J04 3.7 ± 0.3 kilonewton per meter
J08 6.1 ± 0.4 kilonewton per meter

The following laboratories were omitted from the grand means because of extreme test results: 309, 372, 616

Data from the following laboratories appear to be off by a multiplicative factor: 360, 558

ANALYSIS T20-1 TABLE 2


TENSILE BREAKING STRENGTH, KILOGNEWTONS PER METER

TAPPI STANDARD T494 G3-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	F	MEANS		COORDINATES		AVG E.SDR	VAR	PROPERTY	TEST	INSTRUMENT	CONDITIONS
		J04	J08	MAJOR	MINOR						
L372	#	.34	6.09	-1.56	2.94	.77	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L558	#	.96	1.32	-5.48	.15	.70	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L616	#	1.17	.40	-6.19	-0.47	.58	20D	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L360	#	1.26	2.13	-4.63	.26	.37	20B	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L291	*	3.19	5.63	-0.63	.21	1.43	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L251	*	3.20	5.57	-0.68	.17	1.61	20I	TENSILE STRENGTH,	PRINTING PAPER, CRE, 20 C,	65% RH	
L143	Ø	3.36	5.41	-0.74	-0.04	.92	20E	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L176	Ø	3.39	5.64	-0.53	.04	1.02	20E	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L557	Ø	3.40	5.93	-0.26	.16	.89	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L563A	Ø	3.50	5.79	-0.34	.02	1.86	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L331	Ø	3.50	5.48	-0.62	-0.13	1.20	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L442	Ø	3.51	5.91	-0.23	.05	.77	20G	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L325	Ø	3.52	5.90	-0.24	.05	1.15	20E	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L315	Ø	3.52	5.63	-0.47	-0.08	1.00	20G	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L124C	Ø	3.52	5.82	-0.31	.01	1.15	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L559	Ø	3.52	6.17	.00	.17	.58	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L105	*	3.55	6.46	.27	.28	1.32	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L352	Ø	3.56	5.84	-0.27	-0.02	1.23	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L260	Ø	3.57	6.06	-0.07	.08	.71	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L278	Ø	3.60	6.15	.02	.10	.89	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L315	Ø	3.61	6.07	-0.04	.05	1.00	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L100	Ø	3.62	6.22	.10	.11	.75	20E	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L190R	Ø	3.64	6.02	-0.08	-0.01	.90	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L328	Ø	3.65	5.89	-0.18	-0.07	.92	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L592	Ø	3.66	6.10	.01	.02	.87	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L139	*	3.72	6.02	-0.04	-0.08	.99	20H	TENSILE STRENGTH,	PRINTING PAPER, CRE, SHORT	TEST SPAN	
L378	Ø	3.73	5.75	-0.27	-0.21	1.31	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L223R	Ø	3.73	6.25	.17	.03	.81	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L185	Ø	3.73	6.30	.21	.05	1.06	20C	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L148	Ø	3.74	5.99	-0.06	-0.11	.83	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L587	M	3.75				1.05	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L333	Ø	3.75	6.13	.07	-0.05	1.02	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L141T	Ø	3.78	6.16	.11	-0.06	.84	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L243	Ø	3.79	6.09	.05	-0.10	.90	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L344	Ø	3.79	6.03	.00	-0.13	1.20	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L618	Ø	3.79	6.10	.06	-0.10	1.24	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L159	Ø	3.79	6.22	.17	-0.04	.90	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L230	Ø	3.80	6.45	.38	.06	.70	20G	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L261	Ø	3.80	6.41	.34	.04	.95	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L163	Ø	3.81	6.41	.35	.03	.77	20D	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L255	Ø	3.82	6.33	.29	-0.01	.63	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L390	Ø	3.83	6.37	.32	-0.01	1.08	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L575	Ø	3.84	6.46	.40	.03	.84	20G	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L125	Ø	3.86	6.17	.16	-0.13	1.45	20C	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L122	Ø	3.89	6.27	.27	-0.11	.96	20A	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L226C	Ø	3.92	6.40	.39	-0.07	1.69	20C	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L131	Ø	3.97	6.54	.54	-0.05	.76	20E	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L167	Ø	4.02	6.67	.68	-0.03	1.31	20G	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
L309	#	20.39	5.64	7.49	-14.96	51.08	20E	TENSILE STRENGTH,	PRIMARYLY PRINTING PAPERS,	LOAD CELL (CRE)	
GMEANS:		3.67	6.09			1.00					
95% ELLIPSE:				.85	.26	WITH GAMMA = 61 DEGREES					

TENSILE STRENGTH, CRE TYPE

SAMPLE J04 = 3.67 KILONEWTON/M SAMPLE J08 = 6.09 KILONEWTON/M
 SAMPLE J04 = 12.39 LB/15 MM SAMPLE J08 = 20.53 LB/15 MM

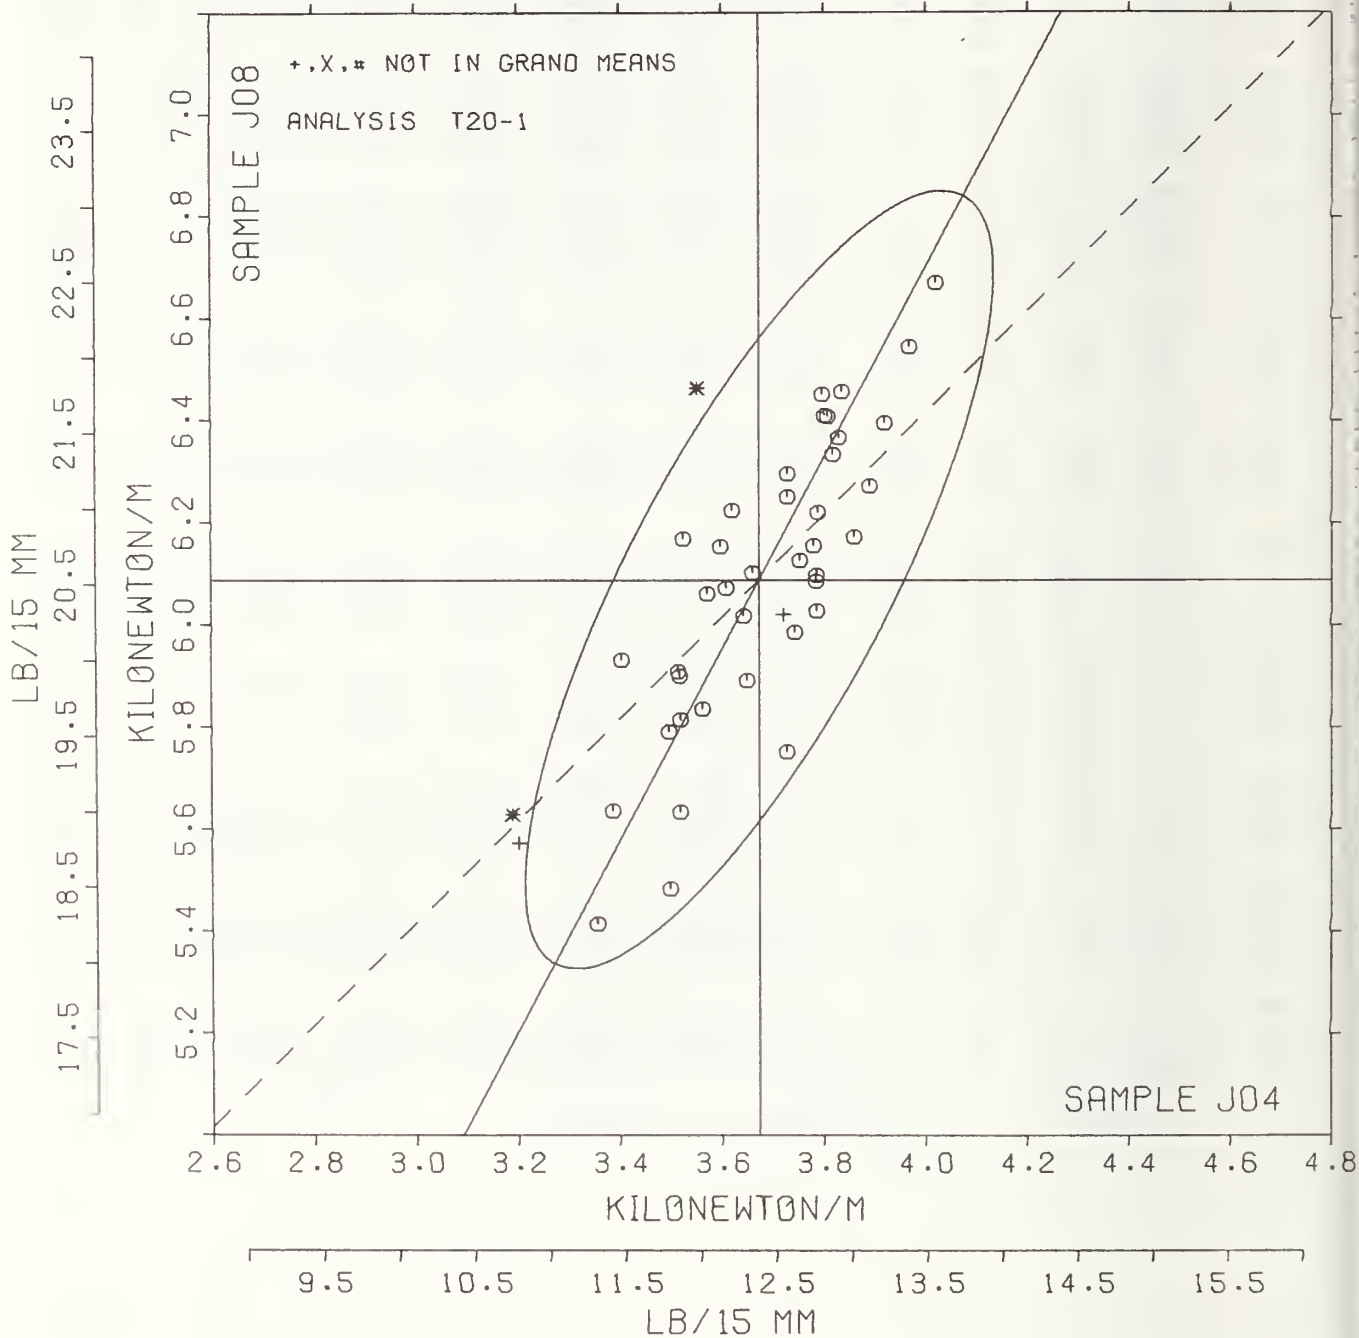

TENSILE BREAKING STRENGTH, KILOWEIGHTS PER METER
TAPPI STANDARD T404 69-76, TENSILE BREAKING STRENGTH OF PAPER AND PAPERBOARD (PENDULUM-TYPE TESTER)

LAB CODE	SAMPLE J04 MEAN	PRINTING 73 GRAMS PER SQUARE METER				SAMPLE J08 MEAN	PRINTING 85 GRAMS PER SQUARE METER				TEST D. ° 20		
		DEV	N.DEV	SDR	R.SDR		DEV	N.DEV	SDR	R.SDR	VAR	F	LAB
L103	3.88	.12	.59	.12	.60	6.48	.25	.64	.25	.58	20R	Ø	L103
L108	3.70	-.05	-.24	.19	.93	6.50	.28	.70	.18	.43	20P	Ø	L108
L121	3.90	.15	.69	.16	.79	6.28	.05	.14	.51	1.19	20P	Ø	L121
L124P	3.54	-.21	-.99	.23	1.12	5.93	-.30	-.74	.44	1.02	20P	Ø	L124P
L128	3.81	.05	.26	.13	.63	6.34	.12	.29	.41	.96	20T	Ø	L128
L148	3.73	-.02	-.10	.17	.83	6.03	-.19	-.48	.27	.63	20P	Ø	L148
L162	3.47	-.28	-1.34	.30	1.45	6.20	-.03	-.07	.36	.85	20*	Ø	L162
L182L	3.69	-.07	-.31	.20	.96	6.07	-.15	-.38	.51	1.19	20T	Ø	L182L
L189	4.06	.30	1.44	.18	.87	6.83	.61	1.52	.62	1.45	20R	Ø	L189
L191P	3.90	.15	.69	.19	.94	6.50	.27	.69	.35	.82	20P	Ø	L191P
L195	3.83	.08	.38	.16	.79	6.17	-.06	-.14	.28	.66	20R	Ø	L195
L211	2.81	-.94	-4.46	.21	1.00	4.99	-1.23	-3.10	.28	.65	20R	#	L211
L212	3.28	-.47	-2.22	.25	1.20	5.53	-.70	-1.75	.31	.72	20R	Ø	L212
L213	3.51	-.24	-1.15	.22	1.08	6.22	-.01	-.01	.39	.92	20T	Ø	L213
L218	3.81	.05	.26	.15	.71	6.33	.11	.27	.32	.74	20P	Ø	L218
L242	3.70	-.05	-.25	.18	.85	5.66	-.56	-1.40	.63	1.47	20Y	Ø	L242
L249	3.64	-.12	-.56	.19	.93	5.96	-.26	-.66	.67	1.57	20P	Ø	L249
L259	4.00	.25	1.16	.19	.91	6.30	.08	.19	.59	1.38	20P	Ø	L259
L262	3.82	.07	.32	.20	.96	6.88	.66	1.65	.24	.56	20R	Ø	L262
L275	3.68	-.08	-.37	.28	1.33	6.47	.24	.61	.54	1.27	20R	Ø	L275
L279P	3.84	.09	.42	.47	2.28	6.85	.62	1.56	.42	.98	20P	Ø	L279P
L285	3.50	-.26	-1.21	.14	.67	4.77	-1.45	-3.65	.16	.37	20P	#	L285
L311	3.78	.03	.15	.18	.88	5.51	-.71	-1.78	.39	.91	20V	Ø	L311
L330	3.69	-.07	-.31	.21	1.01	6.22	-.00	-.00	.55	1.28	20P	Ø	L330
L356	4.02	.27	1.26	.16	.79	6.45	.23	.58	.56	1.30	20P	Ø	L356
L362	3.75	-.01	-.03	.29	1.42	6.32	.09	.23	.39	.91	20R	Ø	L362
L370	3.79	.03	.16	.12	.58	6.46	.24	.60	.39	.90	20P	Ø	L370
L376	3.68	-.07	-.32	.18	.88	5.72	-.51	-1.28	.55	1.28	20P	Ø	L376
L393	3.95	.19	.92	.15	.73	6.46	.24	.60	.37	.86	20P	Ø	L393
L484	3.53	-.22	-1.04	.25	1.19	5.51	-.71	-1.79	.55	1.28	20U	Ø	L484
L554	3.98	.23	1.09	.22	1.06	6.75	.53	1.32	.32	.74	20P	Ø	L554
L556	4.13	.38	1.79	.20	.95	6.27	.04	.11	.66	1.55	20P	Ø	L556
L563P	4.04	.29	1.36	.20	.95	6.78	.56	1.39	.49	1.14	20P	Ø	L563P
L585	3.32	-.44	-2.07	.15	.73	5.71	-.51	-1.28	.30	.69	20V	Ø	L585
L599	3.40	-.35	-1.65	.35	1.69	5.70	-.52	-1.31	.32	.75	20V	Ø	L599

GR. MEAN = 3.75 KILOWEIGHT/M GRAND MEAN = 6.22 KILOWEIGHT/M TEST DETERMINATIONS = 20
SD MEANS = .21 KILOWEIGHT/M SD OF MEANS = .40 KILOWEIGHT/M 33 LABS IN GRAND MEANS
AVERAGE SDR = .21 KILOWEIGHT/M AVERAGE SDR = .43 KILOWEIGHT/M

GR. MEAN = 12.660 LB/15 MM GRAND MEAN = 20.989 LB/15 MM
TOTAL NUMBER OF LABORATORIES REPORTING = 35

Best values: J04 3.7 ± 0.4 kilonewton per meter
J08 6.3 ± 0.6 kilonewton per meter

The following laboratories were omitted from the grand means because of extreme test results: 211, 285


TENSILE BREAKING STRENGTH, KILONEWTONS PER METER

TAPPI STANDARD T404 68-76, TENSILE BREAKING STRENGTH OF PAPER AND PAPERBOARD (PENDULUM-TYPE TESTER)

LAB CODE	P	MEANS		COORDINATES		AVG		PROPERTY==TEST	INSTRUMENT===CONDITIONS
		J04	J08	MAJOR	MINOR	R.SDR	VAR		
L211	#	2.81	4.99	-1.50	.40	.82	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L212	Ø	3.28	5.53	-.82	.17	.96	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L585	Ø	3.32	5.71	-.64	.21	.71	20V	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L599	Ø	3.40	5.70	-.62	.12	1.22	20V	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L162	Ø	3.47	6.20	-.13	.25	1.15	20*	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L285	#	3.50	4.77	-1.44	-.32	.52	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L213	Ø	3.51	6.22	-.10	.22	1.00	20T	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L484	Ø	3.53	5.51	-.74	-.07	1.23	20U	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L124P	Ø	3.54	5.93	-.35	.08	1.07	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L249	Ø	3.64	5.96	-.29	.01	1.25	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L275	Ø	3.68	6.47	.19	.17	1.30	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L376	Ø	3.68	5.72	-.50	-.13	1.08	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L162L	Ø	3.69	6.07	-.17	.00	1.07	20T	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L33C	Ø	3.69	6.22	-.03	.06	1.15	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L242	Ø	3.70	5.66	-.54	-.17	1.16	20Y	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L108	Ø	3.70	6.50	.24	.15	.68	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L148	Ø	3.73	6.03	-.18	-.05	.73	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L362	Ø	3.75	6.32	.08	.04	1.16	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L311	Ø	3.78	5.51	-.64	-.30	.89	20V	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L370	Ø	3.79	6.46	.23	.06	.74	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L128	Ø	3.81	6.34	.13	-.01	.80	20T	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L218	Ø	3.81	6.33	.12	-.01	.72	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L262	Ø	3.82	6.88	.63	.19	.76	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L195	Ø	3.83	6.17	-.02	-.10	.72	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L279P	Ø	3.84	6.85	.61	.15	1.63	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L103	Ø	3.88	6.48	.28	-.02	.59	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L191P	Ø	3.90	6.50	.31	-.03	.88	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L121	Ø	3.90	6.28	.11	-.11	.99	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L393	Ø	3.95	6.46	.30	-.09	.80	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L554	Ø	3.98	6.75	.57	-.01	.90	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L259	Ø	4.00	6.30	.16	-.20	1.15	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L356	Ø	4.02	6.45	.31	-.16	1.04	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L563P	Ø	4.04	6.78	.62	-.05	1.04	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L185	Ø	4.06	6.83	.68	-.05	1.16	20R	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
L556	Ø	4.13	6.27	.18	-.33	1.25	20P	TENSILE STRENGTH,	PRIMARILY PRINTING PAPERS, PENDULUM TESTER
GMEANS:		3.75	6.22			1.00			
		95% ELLIPSE:	1.11	.38		WITH GAMMA = 67 DEGREES			

TENSILE STRENGTH, PENDULUM TYPE

SAMPLE J04 = 3.75 KILONEWTON/M SAMPLE J08 = 6.22 KILONEWTON/M
 SAMPLE J04 = 12.7 LB/15 MM SAMPLE J08 = 21.0 LB/15 MM

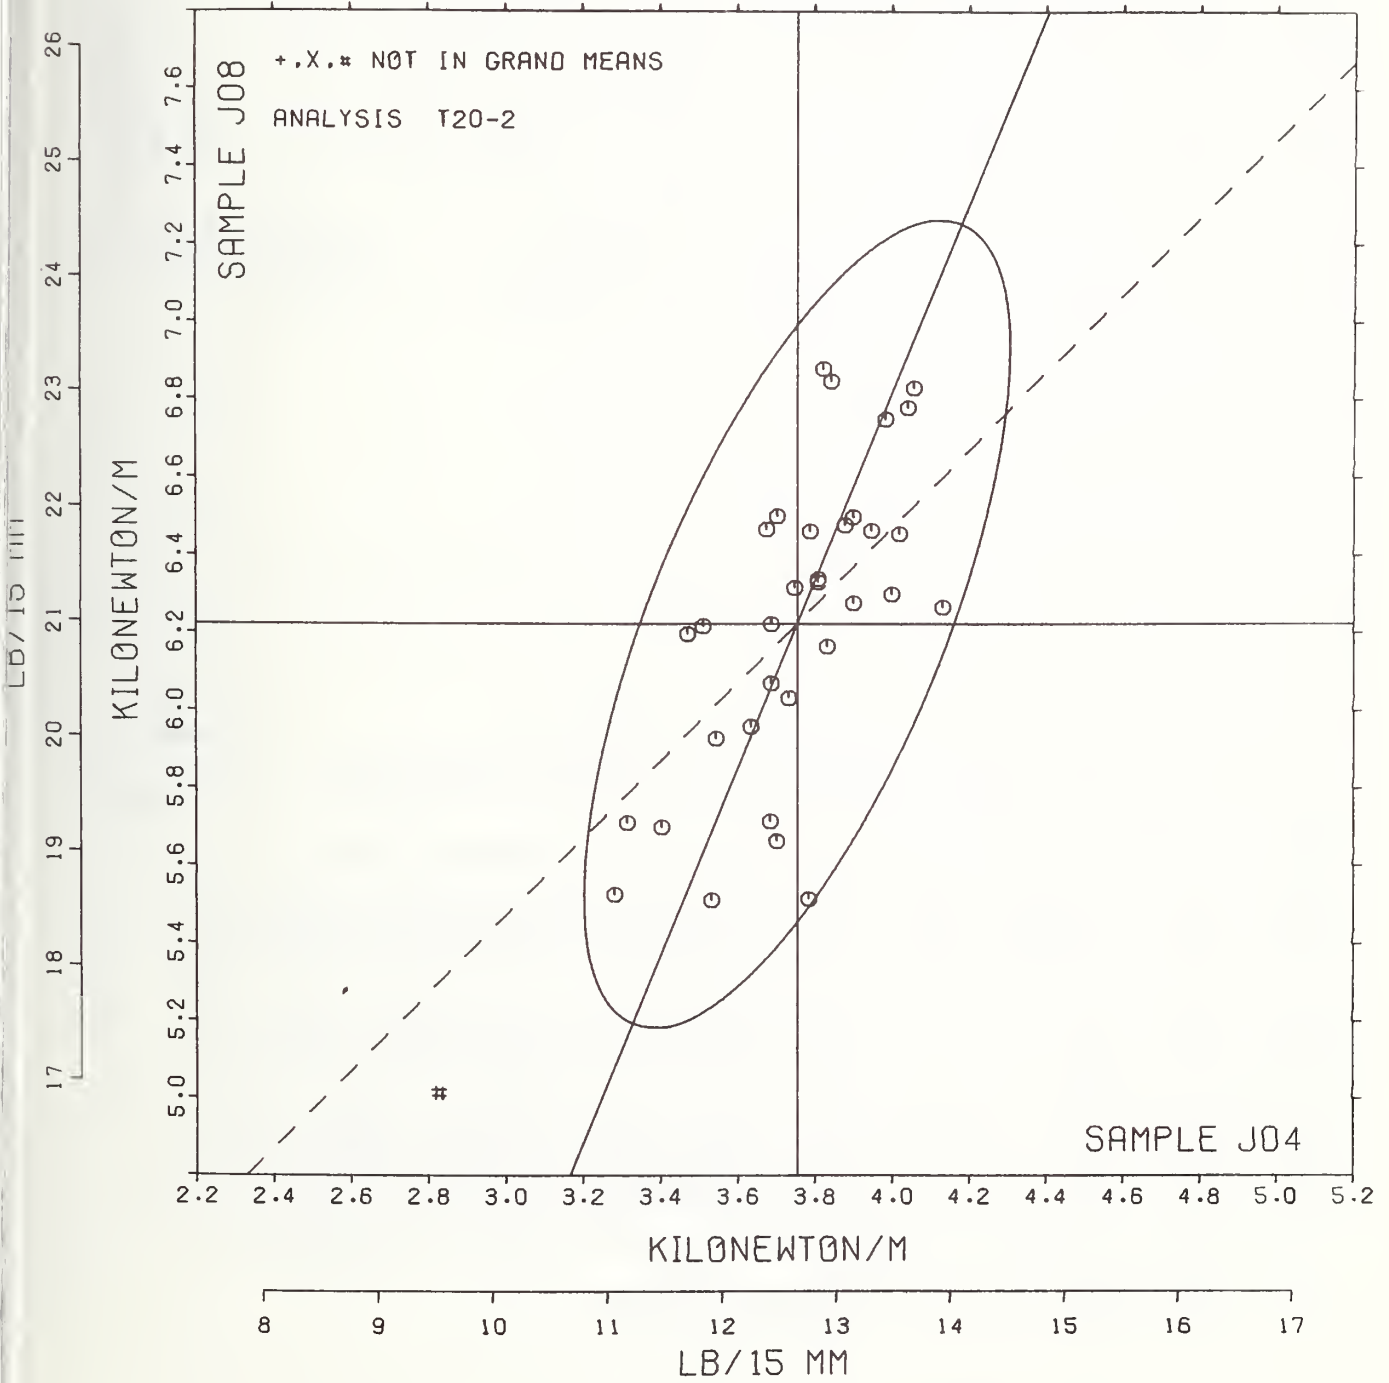

TENSILE ENERGY ABSORPTION, JOULES PER SQUARE METER - PACKAGING PAPER
TAPPI STANDARD T494 G9-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	SAMPLE J15 MEAN	PRINTING 149 GRAMS PER SQUARE METER				R _s SDR	SAMPLE K31 MEAN	PRINTING 105 GRAMS PER SQUARE METER				TEST D. = 20		
		DEV	N _s DEV	SDR	R _s SDR			DEV	N _s DEV	SDR	R _s SDR	VAR	F	LAB
L122	132.2	10.5	.93	11.3	.90	80.2	4.1	.51	9.5	.94	25P	Ø	L122	
L126	121.1	9.5	0.05	9.1	.73	76.6	.5	.07	9.9	.98	25G	Ø	L126	
L151	124.6	3.0	.27	17.4	1.39	82.5	6.4	.81	13.4	1.32	25F	Ø	L151	
L182	115.3	6.4	0.56	10.7	.85	71.5	4.6	0.58	9.1	.90	25B	Ø	L182	
L234B	123.0	1.4	.12	14.8	1.18	87.3	11.2	1.40	11.4	1.12	25H	Ø	L234B	
L237B	107.5	14.1	1.24	10.7	.86	69.2	7.0	0.87	10.1	1.00	25H	Ø	L237B	
L243	120.0	1.7	0.15	9.0	.72	74.2	1.9	0.23	6.9	.68	25Z	Ø	L243	
L264	111.1	10.5	0.93	15.6	1.24	66.5	9.6	1.20	10.4	1.03	25F	Ø	L264	
L267	124.7	3.0	.27	11.8	.94	83.2	7.1	.89	7.7	.76	25F	Ø	L267	
L273	136.4	14.8	1.30	13.1	1.04	85.6	9.5	1.19	10.3	1.02	25F	Ø	L273	
L280	106.7	14.9	1.31	18.4	1.47	69.4	6.7	0.84	12.8	1.26	25B	Ø	L280	
L312	147.1	25.4	2.24	12.3	.98	87.5	11.4	1.43	10.8	1.07	25J	Ø	L312	
L318	129.3	7.7	.68	12.1	.97	76.4	.3	.03	8.6	.85	25A	Ø	L318	
L580	115.6	6.0	0.53	11.7	.93	68.1	8.0	1.00	6.1	.61	25C	Ø	L580	
L604	87.2	34.4	3.03	14.8	1.18	72.0	4.2	0.52	12.4	1.23	25A	#	L604	
L676	109.9	11.7	1.03	10.0	.80	63.3	12.8	1.60	14.7	1.46	25F	Ø	L676	

GR. MEAN = 121.6 JOULES/SQ M GRAND MEAN = 76.1 JOULES/SQ M TEST DETERMINATIONS = 20
SD MEANS = 11.3 JOULES/SQ M SD OF MEANS = 8.0 JOULES/SQ M 15 LABS IN GRAND MEANS
AVERAGE SDR = 12.5 JOULES/SQ M AVERAGE SDR = 10.1 JOULES/SQ M
GR. MEAN = 8.332 FT. LB/SQ FT GRAND MEAN = 5.214 FT. LB/SQ FT
TOTAL NUMBER OF LABORATORIES REPORTING = 16
Best values: J15 120 ± 16 joules per square meter
K31 76 ± 11 joules per square meter


The following laboratories were omitted from the grand means because of extreme test results: 604

TENSILE ENERGY ABSORPTION, JOULES PER SQUARE METER - PACKAGING PAPER
TAPPI STANDARD T494 G9-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY	TEST INSTRUMENT	CONDITIONS
		J15	K31	MAJOR	MINOR	R _s SDR	VAR			
L604	#	87.2	72.0	-31.0	15.5	1.20	25A	TENSILE ENERGY ABS.	PACKAGING PAPER, PLAT/FLAT JAWS	
L280	Ø	106.7	69.4	-16.1	2.6	1.36	25B	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
L237B	Ø	107.5	69.2	-15.6	1.9	.93	25H	TENSILE ENERGY ABS.	PACKAGING PAPER, 2-PIN STRAIN GAGE	
L676	Ø	109.9	63.3	-16.8	4.2	1.13	25F	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
L264	Ø	111.1	66.5	-14.1	2.2	1.13	25F	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
L182	Ø	115.3	71.5	-7.8	0.4	.88	25B	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
L580	Ø	115.6	68.1	-9.4	3.4	.77	25C	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/LINE JAWS	
L243	Ø	120.0	74.2	-2.4	0.6	.70	25Z	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/LINE JAWS	
L126	Ø	121.1	76.6	0.1	.7	.85	25G	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/LINE JAWS	
L234B	Ø	123.0	87.3	7.3	8.6	1.15	25H	TENSILE ENERGY ABS.	PACKAGING PAPER, 2-PIN STRAIN GAGE	
L151	Ø	124.6	82.5	6.1	3.7	1.36	25F	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
L267	Ø	124.7	83.2	6.4	4.3	.85	25F	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
L318	Ø	129.3	76.4	6.5	4.0	.91	25A	TENSILE ENERGY ABS.	PACKAGING PAPER, FLAT/FLAT JAWS	
L122	Ø	132.2	80.2	11.0	2.4	.92	25P	TENSILE ENERGY ABS.	PACKAGING PAPER, PATTERNED FLAT JAWS	
L273	Ø	136.4	85.6	17.5	0.2	1.03	25F	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
L312	Ø	147.1	87.5	27.5	4.4	1.03	25J	TENSILE ENERGY ABS.	PACKAGING PAPER, LINE/FLAT JAWS	
GMEANS:		121.6	76.1			1.00				
		95% ELLIPSE:		38.3	10.6	WITH GAMMA = 33 DEGREES				

T.E.A., PACKAGING PAPERS

SAMPLE J15 = 122. JOULES/SQ M SAMPLE K31 = 76. JOULES/SQ M
 SAMPLE J15 = 8.33 FT.LB/SQ FT SAMPLE K31 = 5.21 FT.LB/SQ FT

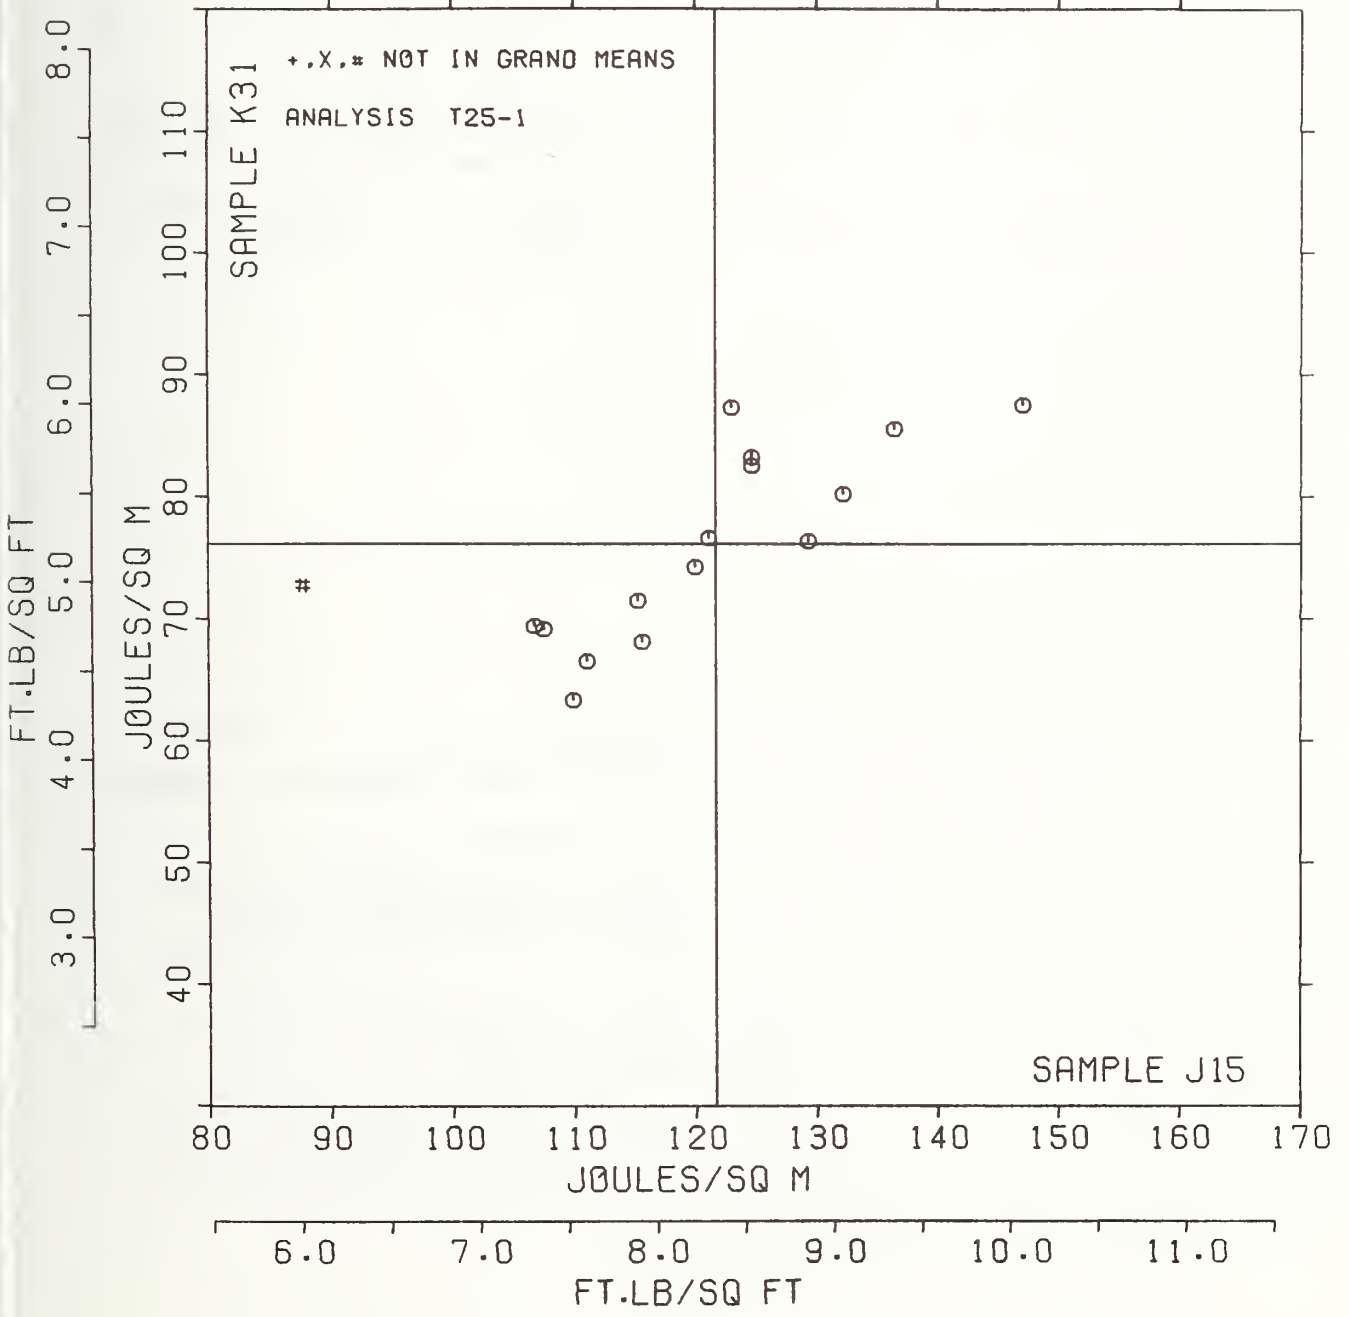

TENSILE ENERGY ABSORPTION, JOULES PER SQUARE METER - PRINTING PAPER
TAPPI STANDARD T494 6S-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	SAMPLE J04		PRINTING 73 GRAMS PER SQUARE METER				SAMPLE J08		PRINTING 85 GRAMS PER SQUARE METER				TEST D. = 20		
	MEAN	DEV	N.DEV	SDR	R.SDR	MEAN	DEV	N.DEV	SDR	R.SDR	VAR	F	LAB		
L100	34.8	-2.9	-1.12	3.9	.96	78.0	2.1	.32	6.1	.82	26A	Ø	L100		
L122	39.9	2.2	.84	3.5	.87	79.2	3.4	.51	10.8	1.44	26L	Ø	L122		
L139	36.0	-1.8	-.68	5.9	1.46	68.6	-7.3	-1.09	7.6	1.03	26H	Ø	L139		
L159	40.3	2.6	1.00	4.2	1.04	82.0	6.2	.93	8.6	1.15	26F	Ø	L159		
L163	36.5	-1.2	-.48	4.1	1.01	78.9	3.1	.46	5.5	.73	26J	Ø	L163		
L167	40.2	2.5	.97	2.2	.54	66.7	-9.1	-1.37	5.0	.67	26D	Ø	L167		
L185	34.5	-3.2	-1.24	5.4	1.34	69.9	-5.9	-.89	7.8	1.04	26C	Ø	L185		
L255	43.2	5.5	2.14	3.3	.82	87.3	11.4	1.72	5.9	.80	26P	Ø	L255		
L309	38.2	.5	.21	5.5	1.35	69.8	-6.0	-.90	5.4	.72	26J	Ø	L309		
L318	38.4	.7	.26	3.5	.87	72.2	-3.6	-.54	10.9	1.46	26A	Ø	L318		
L393	36.3	-1.4	-.54	3.5	.87	80.8	5.0	.75	5.0	.67	26V	Ø	L393		
L442	38.6	.9	.34	3.8	.93	81.7	5.9	.89	9.2	1.23	26B	Ø	L442		
L575	36.6	-1.1	-.43	4.5	1.11	79.8	4.0	.60	7.4	1.00	26A	Ø	L575		
L587	35.4	-2.3	-.91	5.0	1.24	NO DATA REPORTED FOR SAMPLE J08					26C	Ø	L587		
L592	34.5	-3.3	-1.27	3.4	.85	66.6	-9.2	-1.38	9.2	1.24	26H	Ø	L592		


GR. MEAN = 37.7 JOULES/SQ M GRAND MEAN = 75.8 JOULES/SQ M TEST DETERMINATIONS = 20
SD MEANS = 2.6 JOULES/SQ M SD OF MEANS = 6.6 JOULES/SQ M 14 LABS IN GRAND MEANS
AVERAGE SDR = 4.1 JOULES/SQ M AVERAGE SDR = 7.4 JOULES/SQ M
GR. MEAN = 2.584 FT.LB/SQ FT GRAND MEAN = 5.194 FT.LB/SQ FT
TOTAL NUMBER OF LABORATORIES REPORTING = 15
Best values: J04 38 ± 5 joules per square meter
J08 76 ± 10 joules per square meter

TENSILE ENERGY ABSORPTION, JOULES PER SQUARE METER - PRINTING PAPER
TAPPI STANDARD T494 6S-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY	TEST INSTRUMENT	CONDITIONS
		J04	J08	MAJOR	MINOR	R.SDR	VAR			
L592	Ø	34.5	66.6	-9.6	1.4	1.04	26H	TENSILE ENERGY ABS.	PRINTING PAPERS,	2-PIN STRAIN GAGE
L185	Ø	34.5	69.9	-6.4	1.9	1.19	26C	TENSILE ENERGY ABS.	PRINTING PAPERS,	LINE/LINE JAWS
L100	Ø	34.8	78.0	1.5	3.2	.89	26A	TENSILE ENERGY ABS.	PRINTING PAPERS,	PLAT/PLAT JAWS
L587	M	35.4				1.24	26C	TENSILE ENERGY ABS.	PRINTING PAPERS,	LINE/LINE JAWS
L139	Ø	36.0	68.6	-7.5	.3	1.24	26H	TENSILE ENERGY ABS.	PRINTING PAPERS,	2-PIN STRAIN GAGE
L393	Ø	36.3	80.8	4.6	2.3	.77	26V	TENSILE ENERGY ABS.	PRINTING PAPERS,	LINE/FLAT JAWS
L163	Ø	36.5	78.9	2.8	1.8	.87	26J	TENSILE ENERGY ABS.	PRINTING PAPERS,	LINE/FLAT JAWS
L575	Ø	36.6	79.8	3.7	1.9	1.05	26A	TENSILE ENERGY ABS.	PRINTING PAPERS,	FLAT/PLAT JAWS
L309	Ø	38.2	69.8	-5.8	-1.7	1.03	26J	TENSILE ENERGY ABS.	PRINTING PAPERS,	LINE/PLAT JAWS
L318	Ø	38.4	72.2	-3.4	-1.4	1.17	26A	TENSILE ENERGY ABS.	PRINTING PAPERS,	FLAT/FLAT JAWS
L442	Ø	38.6	81.7	6.0	.3	1.08	26B	TENSILE ENERGY ABS.	PRINTING PAPERS,	LINE/PLAT JAWS
L122	Ø	39.9	79.2	3.7	-1.4	1.16	26L	TENSILE ENERGY ABS.	PRINTING PAPERS,	PATTERNED FLAT JAWS
L167	Ø	40.2	66.7	-8.5	-4.2	.60	26D	TENSILE ENERGY ABS.	PRINTING PAPERS,	2-PIN STRAIN GAGE
L159	Ø	40.3	82.0	6.6	-1.3	1.10	26F	TENSILE ENERGY ABS.	PRINTING PAPERS,	LINE/FLAT JAWS
L255	Ø	43.2	87.3	12.3	-3.1	.81	26P	TENSILE ENERGY ABS.	PRINTING PAPERS,	PATTERNED FLAT JAWS
GMEANS:		37.7	75.8			1.00				
		95% ELLIPSE:		19.6	6.5	WITH GAMMA = 78 DEGREES				

T.E.A., PRINTING PAPERS

SAMPLE J04 = 37.7 JOULES/SQ M SAMPLE J08 = 75.8 JOULES/SQ M
 SAMPLE J04 = 2.58 FT.LB/SQ FT SAMPLE J08 = 5.19 FT.LB/SQ FT

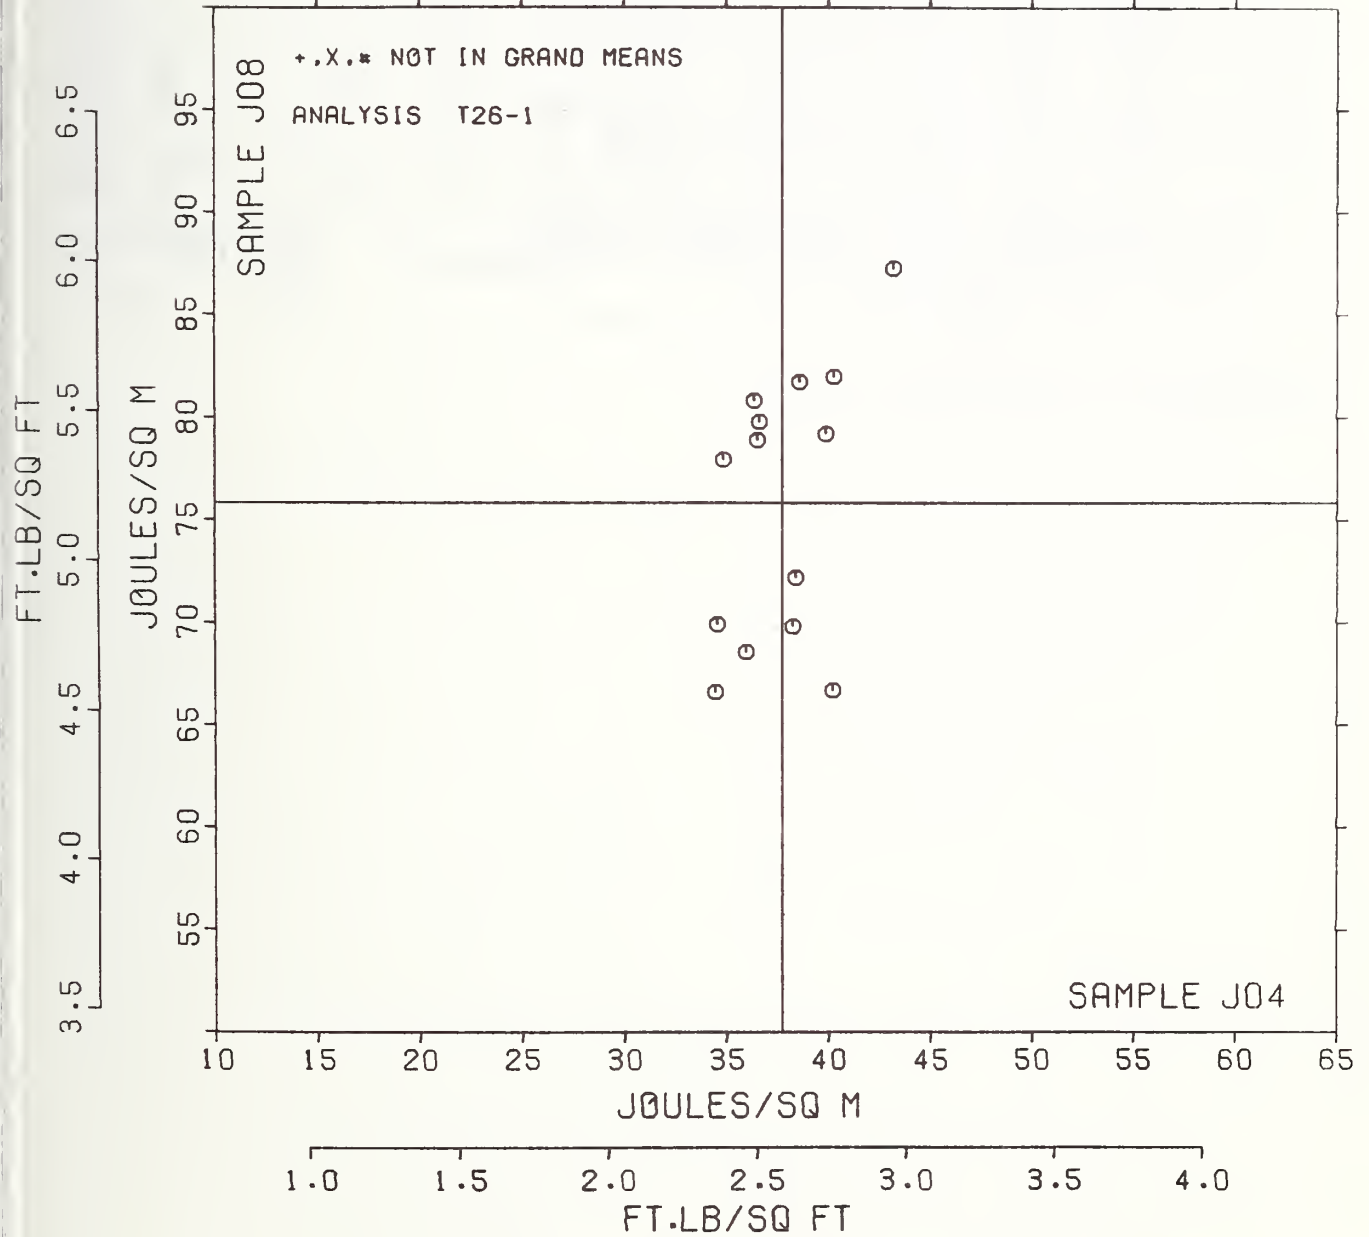


ELONGATION TO BREAK, PERCENT - PACKAGING PAPER
TAPPI STANDARD T494 68-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	P	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---	CONDITIONS
		J15	K31	MAJOR	MINOR	R. SDR	VAR		
L100	Ø	2.005	1.375	-.138	.017	.83	28A	ELONGATION, PACKAGING PAPER, LOAD	CELL, PLAT/FLAT JAWS
L324	Ø	2.020	1.390	-.117	.018	.65	28P	ELONGATION, PACKAGING PAPER, LOAD	CELL, PATTERNED FLAT JAWS
L265	Ø	2.034	1.522	-.016	.105	.99	28A	ELONGATION, PACKAGING PAPER, LOAD	CELL, PLAT/PLAT JAWS
L580	Ø	2.055	1.415	-.074	.012	1.16	28C	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/LINE JAWS
L243	Ø	2.084	1.354	-.094	-.052	.67	28C	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/LINE JAWS
L264	Ø	2.085	1.405	-.059	-.015	1.38	28B	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/FLAT JAWS
L126	Ø	2.056	1.421	-.040	-.011	.90	28C	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/LINE JAWS
L182	Ø	2.056	1.376	-.071	-.044	.91	28B	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/PLAT JAWS
L336	Ø	2.124	1.461	.008	-.001	1.28	28A	ELONGATION, PACKAGING PAPER, LOAD	CELL, PLAT/PLAT JAWS
L582	Ø	2.167	1.517	.077	.010	1.19	28A	ELONGATION, PACKAGING PAPER, LOAD	CELL, PLAT/FLAT JAWS
L267	Ø	2.200	1.554	.127	.015	.86	28B	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/FLAT JAWS
L581	Ø	2.208	1.577	.148	.025	.93	28A	ELONGATION, PACKAGING PAPER, LOAD	CELL, PLAT/FLAT JAWS
L280	Ø	2.219	1.554	.141	.002	1.40	28B	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/FLAT JAWS
L122	Ø	2.253	1.473	.110	-.081	.87	28P	ELONGATION, PACKAGING PAPER, LOAD	CELL, PATTERNED FLAT JAWS
L151	#	2.280	1.860	.394	.183	1.85	28B	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/PLAT JAWS
L318	#	2.464	1.546	.314	-.172	.92	28A	ELONGATION, PACKAGING PAPER, LOAD	CELL, PLAT/FLAT JAWS
L312	#	2.565	1.750	.527	-.092	1.02	28B	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/FLAT JAWS
L676	#	2.645	2.090	.818	.101	2.88	28B	ELONGATION, PACKAGING PAPER, LOAD	CELL, LINE/FLAT JAWS
GMEANS:		2.118	1.457			1.00			
		95% ELLIPSE:		.294	.125	WITH GAMMA = 43 DEGREES			

ELONGATION TO BREAK, PACKAGING PAPER

SAMPLE J15 = 2.12 PERCENT

SAMPLE K31 = 1.46 PERCENT

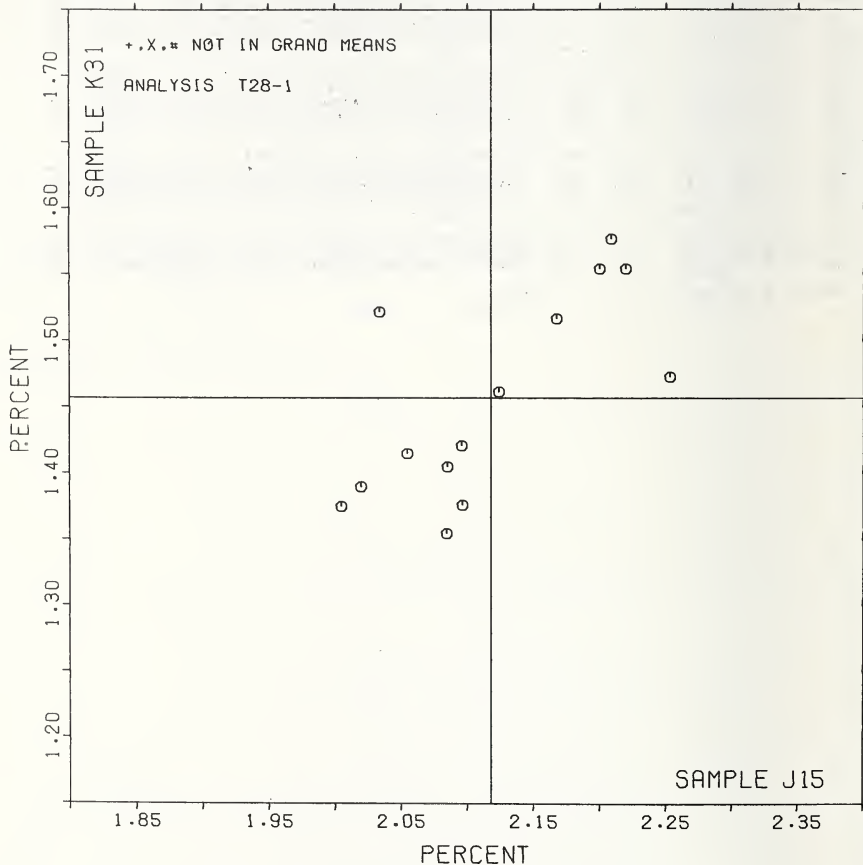

ELONGATION TO BREAK, PERCENT - PRINTING PAPER
TAPPI STANDARD T494 68-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	SAMPLE J04					SAMPLE J08					TEST D. = 20		
	MEAN	73 GRAMS PER SQUARE METER DEV	PRINTING N. DEV	SQR	R. SDR	MEAN	85 GRAMS PER SQUARE METER DEV	PRINTING N. DEV	SQR	R. SDR	VAR	F	LAB
L100	1.470	-.070	-.35	.142	1.19	1.855	.013	.07	.094	.63	29A	0	L100
L105	1.075	-.465	-2.32	.143	1.20	1.437	-.405	-2.22	.197	1.31	29A	0	L105
L122	1.560	.021	.10	.089	.74	1.912	.070	.39	.160	1.06	29F	0	L122
L141T	1.495	-.045	-.22	.107	.90	1.766	-.076	-.42	.140	.93	29D	0	L141T
L176	1.465	-.075	-.37	.179	1.50	1.914	.072	.40	.158	1.05	29B	0	L176
L185	1.454	-.086	-.43	.148	1.24	1.758	-.084	-.46	.111	.74	29C	0	L185
L190R	1.541	.001	.01	.091	.77	1.779	-.063	-.35	.168	1.12	29A	0	L190R
L255	1.785	.245	1.22	.081	.68	2.125	.283	1.55	.089	.59	29F	0	L255
L278	1.592	.052	.26	.132	1.11	1.945	.103	.57	.155	1.03	29A	0	L278
L309	1.778	.238	1.19	.160	1.35	2.042	.200	1.10	.114	.76	29A	0	L309
L318	1.712	.172	.86	.120	1.01	1.979	.137	.76	.157	1.05	29A	0	L318
L344	1.437	-.102	-.51	.138	1.15	1.662	-.180	-.99	.211	1.41	29A	0	L344
L372	1.246	-.294	-1.46	.067	.57	1.513	-.329	-1.81	.223	1.49	29B	0	L372
L378	1.920	.381	1.89	.152	1.28	1.974	.132	.73	.216	1.44	29A	0	L378
L442	1.657	.117	.58	.106	.89	1.987	.145	.80	.130	.87	29B	0	L442
L575	1.497	-.043	-.21	.116	.97	1.904	.062	.34	.131	.87	29A	0	L575
L587	1.460	-.080	-.40	.127	1.07	NO DATA REPORTED FOR SAMPLE J08					29C	M	L587
L592	1.492	-.047	-.24	.089	.75	1.759	-.083	-.45	.163	1.08	29D	0	L592
GR. MEAN	1.540	PERCENT			GRAND MEAN	1.842	PERCENT			TEST DETERMINATIONS	20		
SD MEANS	.201	PERCENT			SD OF MEANS	.182	PERCENT			17 LABS IN GRAND MEANS			
		AVERAGE SDR	.119	PERCENT			AVERAGE SDR	.150	PERCENT				
L242	1.920	.380	1.89	.182	1.53	2.070	.228	1.25	.172	1.15	29R	0	L242
L484	1.460	-.080	-.40	.229	1.92	1.750	-.092	-.50	.238	1.58	29R	0	L484
TOTAL NUMBER OF LABORATORIES REPORTING	= 20												
Best values:	J04	1.50 ± 0.28 percent											
	J08	1.86 ± 0.34 percent											

ANALYSIS T29-1 TABLE 2

ELONGATION TO BREAK, PERCENT - PRINTING PAPER


TAPPI STANDARD T494 GS-70, TENSILE BREAKING PROPERTIES OF PAPER & PAPERBOARD (CONSTANT RATE OF ELONGATION)

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---CONDITIONS
		J04	J08	MAJOR	MINOR	R.SDR	VAR	
L105	Ø	1.075	1.437	-.616	.009	1.25	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L372	Ø	1.246	1.513	-.439	-.049	1.03	29B	ELONGATION, PRINTING PAPERS, LOAD CELL, LINE/FLAT JAWS
L344	Ø	1.437	1.662	-.196	-.065	1.28	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L185	Ø	1.454	1.758	-.120	-.005	.99	29C	ELONGATION, PRINTING PAPERS, LOAD CELL, LINE/LINE JAWS
L484	*	1.460	1.750	-.121	-.015	1.75	29R	ELONGATION, PRINTING PAPERS, PENDULUM, FLAT/FLAT JAWS
L587	M	1.460				1.07	29C	ELONGATION, PRINTING PAPERS, LOAD CELL, LINE/LINE JAWS
L176	Ø	1.465	1.914	-.008	.104	1.28	29B	ELONGATION, PRINTING PAPERS, LOAD CELL, LINE/FLAT JAWS
L100	Ø	1.470	1.855	-.043	.056	.91	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L592	Ø	1.492	1.759	-.090	-.030	.92	29D	ELONGATION, PRINTING PAPERS, LOAD CELL, 2-PIN STRAIN GAGE
L141T	Ø	1.495	1.766	-.084	-.026	.92	29D	ELONGATION, PRINTING PAPERS, LOAD CELL, 2-PIN STRAIN GAGE
L575	Ø	1.497	1.904	.010	.074	.92	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L150E	Ø	1.541	1.779	-.041	-.048	.94	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L122	Ø	1.560	1.912	.062	.039	.90	29P	ELONGATION, PRINTING PAPERS, LOAD CELL, PATTERNED FLAT JAWS
L278	Ø	1.592	1.945	.108	.042	1.07	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L442	Ø	1.657	1.987	.184	.030	.88	29B	ELONGATION, PRINTING PAPERS, LOAD CELL, LINE/FLAT JAWS
L318	Ø	1.712	1.979	.220	-.012	1.03	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L309	Ø	1.778	2.042	.311	-.010	1.05	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
L255	Ø	1.785	2.125	.371	.047	.64	29P	ELONGATION, PRINTING PAPERS, LOAD CELL, PATTERNED FLAT JAWS
L242	*	1.920	2.070	.435	-.084	1.34	29R	ELONGATION, PRINTING PAPERS, PENDULUM, FLAT/FLAT JAWS
L378	*	1.920	1.974	.372	-.155	1.36	29A	ELONGATION, PRINTING PAPERS, LOAD CELL, FLAT/FLAT JAWS
GMEANS:		1.540	1.842			1.00		
		95% ELLIPSE:		.740	.173			WITH GAMMA = 41 DEGREES

ELONGATION TO BREAK, PRINTING PAPER

SAMPLE J04 = 1.54 PERCENT

SAMPLE J08 = 1.84 PERCENT

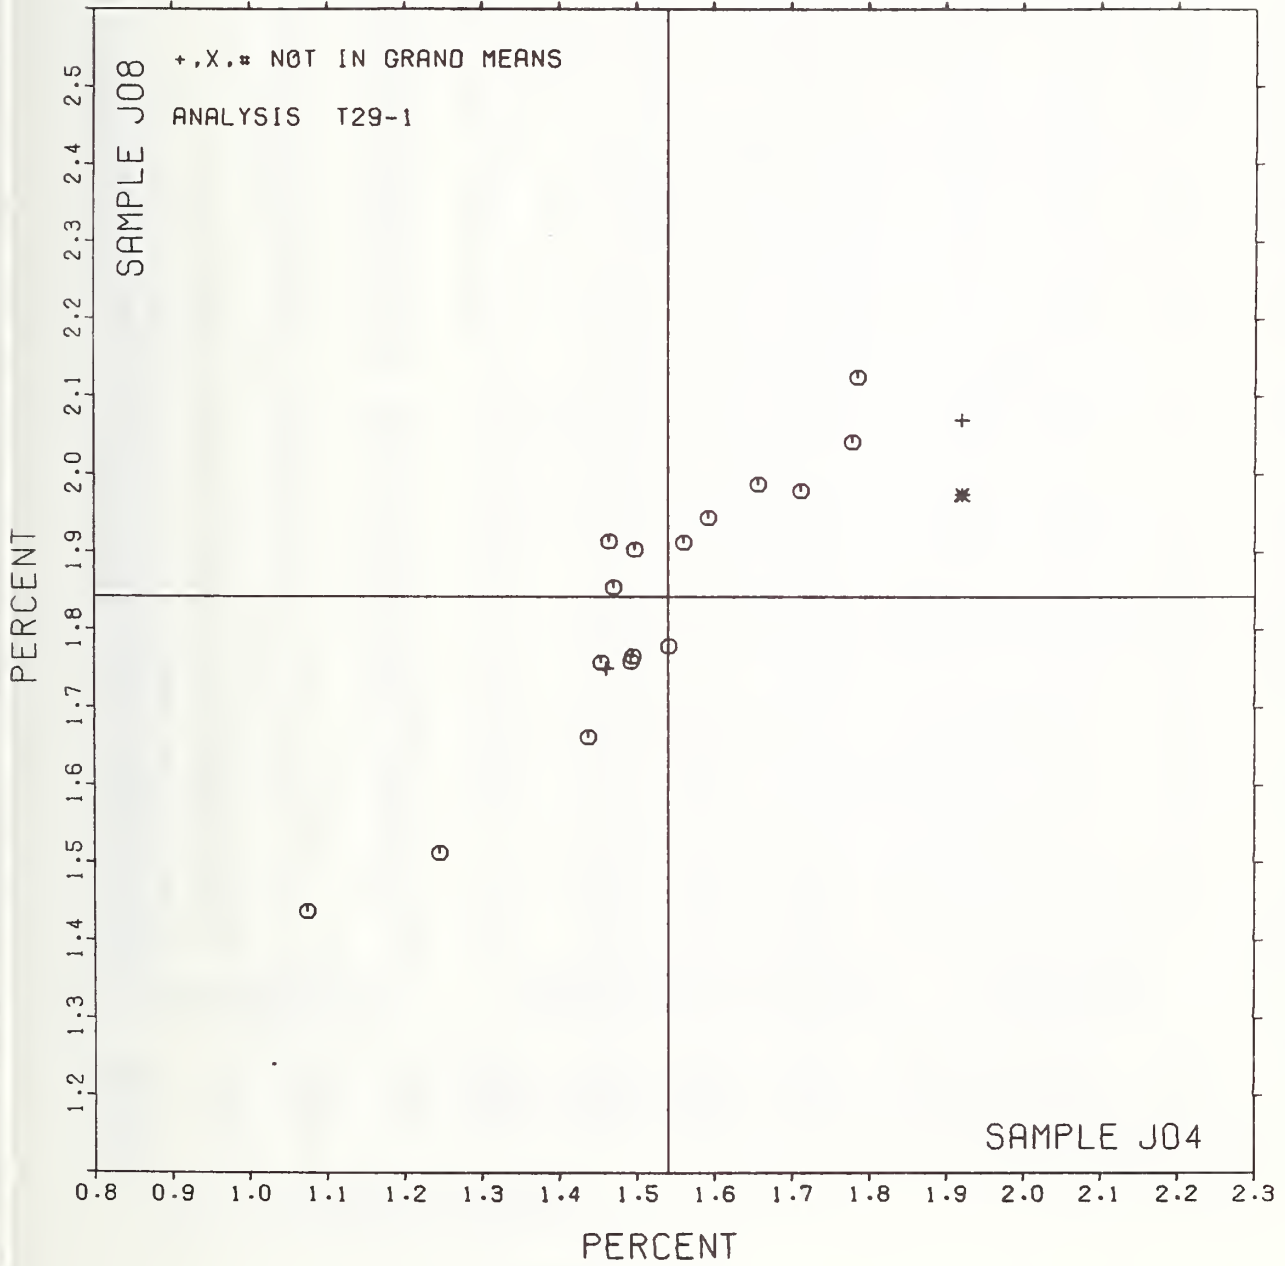

TAPPI COLLABORATIVE REFERENCE PROGRAM
ANALYSIS T30-1 TABLE 1
FOLDING ENDURANCE (MIT), DOUBLE FOLDS
TAPPI STANDARD T511 SU-69

LAB CODE	SAMPLE J29 MEAN	PRINTING 102 GRAMS PER SQUARE METER				SAMPLE J31 MEAN	PRINTING 86 GRAMS PER SQUARE METER				TEST D. = 15			
		DEV	N.DEV	SDR	R.SDR		DEV	N.DEV	SDR	R.SDR	VAR	F	LAB	
L100M	16.4	-7.9	-1.13	4.3	.46	69.1	-3.9	-0.26	12.5	.70	30M	0	L100M	
L100N	15.9	-8.4	-1.20	2.4	.26	77.3	4.3	.29	8.0	.45	30N	0	L100N	
L105	22.2	-2.1	-.29	14.8	1.59	75.2	2.3	.15	9.3	.52	30M	0	L105	
L121	24.5	.2	.03	21.0	2.24	78.6	5.7	.38	15.1	.84	30M	0	L121	
L122	31.8	7.5	1.08	21.5	2.30	68.5	-4.4	-.29	35.3	1.97	30M	0	L122	
L124	28.9	4.7	.67	19.0	2.03	62.7	-10.2	-.68	10.7	.60	30N	0	L124	
L150	30.6	6.3	.91	17.9	1.91	80.4	7.5	.50	22.4	1.26	30M	0	L150	
L159	38.9	14.6	2.09	25.5	2.72	85.4	12.5	.83	21.0	1.17	30M	0	L159	
L162	22.7	-1.6	-.23	12.5	1.33	64.8	-8.1	-.54	22.3	1.24	30M	0	L162	
L163	30.7	6.4	.92	10.4	1.11	55.3	-17.7	-1.17	19.1	1.07	30N	0	L163	
L176	27.0	2.7	.39	5.0	.54	67.9	-5.0	-.33	13.8	.77	30N	0	L176	
L182M	28.5	4.3	.61	22.2	2.37	92.9	19.9	1.32	19.6	1.09	30M	0	L182M	
L185	23.9	-.4	-.06	7.5	.80	81.5	8.5	.57	15.7	.88	30N	0	L185	
L190C	29.3	5.0	.72	4.5	.48	72.1	0.8	-.05	18.7	1.05	30N	0	L190C	
L212	18.8	-5.5	-.78	5.2	.56	62.3	-10.6	-.70	11.4	.64	30M	0	L212	
L223F	21.2	-3.1	-.44	9.0	.97	73.7	.8	.05	16.8	.94	30M	0	L223F	
L230	19.5	-4.8	-.69	5.9	.63	64.9	-8.0	-.53	22.0	1.23	30N	0	L230	
L232	28.0	3.7	.54	7.7	.82	92.9	19.9	1.32	31.6	1.77	30N	0	L232	
L236	18.3	-6.0	-.86	5.3	.57	80.4	7.5	.50	11.2	.63	30N	0	L236	
L238A	21.2	-3.1	-.44	6.0	.64	62.8	-10.1	-.67	25.1	1.40	30N	0	L238A	
L238B	16.0	-8.3	-1.18	5.0	.53	58.0	-14.9	-.99	13.2	.74	30D	0	L238B	
L243	24.3	.0	.00	7.5	.80	93.2	20.3	1.34	18.5	1.03	30D	0	L243	
L254	13.4	-10.9	-1.56	4.3	.46	47.2	-25.7	-1.71	11.9	.66	30M	0	L254	
L262	20.1	-4.1	-.59	6.0	.64	70.3	-2.6	-.17	14.6	.82	30N	0	L262	
L275	18.7	-5.6	-.80	5.9	.63	92.9	20.0	1.33	21.2	1.19	30N	0	L275	
L278	15.6	-8.7	-1.24	2.8	.30	48.1	-24.9	-1.65	12.7	.71	30C	0	L278	
L279	20.3	-4.0	-.57	8.4	.90	50.6	-22.3	-1.48	30.7	1.72	30N	0	L279	
L285A	23.9	-.3	-.05	7.4	.79	81.5	8.6	.57	17.3	.97	30N	0	L285A	
L285B	22.4	-1.9	-.27	7.7	.82	92.1	19.2	1.27	30.9	1.73	30N	0	L285B	
L299	20.8	-3.5	-.49	6.2	.66	79.1	6.1	.41	17.4	.97	30N	0	L299	
L320	43.1	18.9	2.71	33.7	3.61	83.8	10.8	.72	26.2	1.47	30N	*	L320	
L326N	16.3	-7.9	-1.13	4.7	.50	43.7	-29.2	-1.94	14.7	.82	30N	0	L326N	
L339	18.9	-5.3	-.76	4.8	.52	69.0	-3.9	-.26	13.4	.75	30N	0	L339	
L366A	25.7	1.5	.21	6.8	.73	74.0	1.1	.07	25.4	1.42	30N	0	L366A	
L376	16.1	-8.2	-1.17	4.5	.48	56.1	-16.9	-1.12	10.8	.60	30N	0	L376	
L378	23.2	-1.1	-.15	5.7	.61	93.9	20.9	1.39	14.9	.83	30N	0	L378	
L388	22.8	-1.5	-.21	5.2	.55	86.3	13.3	.88	12.5	.70	30N	0	L388	
L390	25.7	1.4	.20	14.3	1.53	72.7	0.2	-.01	29.3	1.64	30N	0	L390	
L393	17.3	-6.9	-.99	3.5	.38	61.1	-11.9	-.79	18.4	1.03	30M	0	L393	
L396M	33.1	8.9	1.27	7.7	.83	113.5	40.5	2.69	24.3	1.36	30N	*	L396M	
L565	28.0	3.7	.54	13.7	1.47	59.4	-13.5	-.90	13.5	.75	30N	0	L565	
L589	35.2	10.9	1.57	22.7	2.43	62.1	-10.8	-.72	9.1	.51	30N	0	L589	
L599	27.1	2.9	.41	8.8	.94	51.1	18.2	1.21	21.1	1.18	30C	0	L599	
L622	51.1	26.8	3.84	33.6	3.60	86.9	14.0	.93	26.1	1.46	30M	X	L622	
L670	40.9	16.7	2.39	32.4	3.47	60.8	-12.1	-.81	22.5	1.26	30N	*	L670	
GR. MEAN =	24.3	DOUBLE FOLDS				GRAND MEAN =	72.9	DOUBLE FOLDS				TEST DETERMINATIONS = 15		
SD MEANS =	7.0	DOUBLE FOLDS				SD OF MEANS =	15.1	DOUBLE FOLDS				44 LABS IN GRAND MEANS		
		AVERAGE SDR = 9.3						AVERAGE SDR = 17.9				DOUBLE FOLDS		
L182S	25.8	1.5	.22	27.8	2.98	148.9	76.0	5.04	44.7	2.50	30S	*	L182S	
L190D	26.7	2.5	.36	6.9	.74	158.0	85.1	5.65	40.1	2.24	30S	*	L190D	
L280	15.8	-8.5	-1.21	4.0	.43	49.8	-23.1	-1.54	15.3	.86	30K	*	L280	
L326S	22.3	-2.0	-.28	6.0	.64	120.3	47.3	3.14	32.8	1.83	30S	*	L326S	
L396S	23.3	-1.0	-.14	3.7	.39	29.9	-43.1	-2.86	6.8	.38	30T	*	L396S	
TOTAL NUMBER OF LABORATORIES REPORTING = 50														

Best values: J29 23 double folds
J31 75 double folds

The ISO (International Standards Organization) is proposing that MIT folding endurance be reported as the logarithm (to the base 10) of the double fold instead of the double fold as in the past.

Please see page 43 of this report for a demonstration of this proposal.


LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---CONDITIONS
		J29	J31	MAJOR	MINOR	R.SDR	VAR	
L254	Ø	13.4	47.2	-27.3	5.9	.56	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L278	Ø	15.6	48.1	-26.0	3.9	.51	30C	FOLDING ENDURANCE, MIT, CIRCULATING FAN IN CEILING
L280	*	15.8	49.8	-24.3	4.1	.64	30K	FOLDING ENDURANCE, KÖELER-MOLIN
L100N	Ø	15.9	77.3	2.7	9.0	.35	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L238B	Ø	16.0	58.0	-16.2	5.4	.63	30D	FOLDING ENDURANCE, MIT, MODIFIED DRIVE TO REDUCE HEATING
L376	Ø	16.1	56.1	-18.1	5.0	.54	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L326N	Ø	16.3	43.7	-30.2	2.4	.66	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L100M	Ø	16.4	69.1	-5.2	7.0	.58	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L393	Ø	17.3	61.1	-12.9	4.6	.70	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L236	Ø	18.3	80.4	6.2	7.3	.60	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L275	Ø	18.7	92.9	18.6	9.2	.91	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L212	Ø	18.8	62.3	-11.4	3.4	.60	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L339	Ø	18.9	69.0	-4.8	4.5	.63	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L230	Ø	19.5	64.9	-8.7	3.2	.93	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L262	Ø	20.1	70.3	-3.3	3.6	.73	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L279	Ø	20.3	50.6	-22.7	0.2	1.31	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L299	Ø	20.8	79.1	5.4	4.5	.82	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L223F	Ø	21.2	73.7	.2	3.1	.95	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L238A	Ø	21.2	62.8	-10.5	1.1	1.02	30M	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L105	Ø	22.2	75.2	1.8	2.4	1.05	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L326S	*	22.3	120.3	46.2	10.6	1.24	30S	FOLDING ENDURANCE, SCHÖPPER, LEIPZIG
L285B	Ø	22.4	92.1	18.5	5.3	1.28	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L162	Ø	22.7	64.8	-8.3	.1	1.29	30M	FOLDING ENDURANCE, MIT, WITE CENTRIFUGAL FAN
L388	Ø	22.8	86.3	12.8	3.9	.63	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L378	Ø	23.2	93.9	20.4	4.9	.72	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L396S	*	23.3	29.9	-42.5	-6.9	.39	30T	FOLDING ENDURANCE, SCHÖPPER, TMI
L185	Ø	23.9	81.5	8.3	1.9	.84	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L285A	Ø	23.9	81.5	8.4	1.9	.88	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L243	Ø	24.3	93.2	19.9	3.7	.92	30D	FOLDING ENDURANCE, MIT, MODIFIED DRIVE TO REDUCE HEATING
L121	Ø	24.5	78.6	5.6	.8	1.54	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L390	Ø	25.7	72.7	.1	-1.4	1.58	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L366A	Ø	25.7	74.0	1.3	-1.3	1.07	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L182S	*	25.8	148.9	75.0	12.4	2.74	30S	FOLDING ENDURANCE, SCHÖPPER, LEIPZIG
L190D	*	26.7	158.0	84.1	13.2	1.49	30S	FOLDING ENDURANCE, SCHÖPPER, LEIPZIG
L176	Ø	27.0	67.9	-4.4	-3.6	.65	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L599	Ø	27.1	91.1	18.4	.5	1.06	30C	FOLDING ENDURANCE, MIT, CIRCULATING FAN IN CEILING
L232	Ø	28.0	92.9	20.3	0.0	1.29	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L565	Ø	28.0	59.4	-12.6	-6.2	1.11	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L182M	Ø	28.5	92.9	20.4	-0.6	1.73	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L124	Ø	28.9	62.7	-9.2	-6.5	1.32	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L190C	Ø	29.3	72.1	.1	-5.1	.76	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L150	Ø	30.6	80.4	8.5	-4.9	1.58	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L163	Ø	30.7	55.3	-16.2	-9.5	1.09	30M	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L122	Ø	31.8	68.5	-2.9	-8.2	2.13	30M	FOLDING ENDURANCE, MIT, WITH CENTRIFUGAL FAN
L396M	*	33.1	113.5	41.5	-1.3	1.09	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L589	Ø	35.2	62.1	-8.6	-12.7	1.47	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L159	Ø	38.9	85.4	14.9	-12.1	1.95	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L670	*	40.9	60.8	-8.9	-18.6	2.36	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L320	*	43.1	83.8	14.1	-16.6	2.54	30N	FOLDING ENDURANCE, MIT, NO CENTRIFUGAL FAN
L622	X	51.1	86.9	18.7	-23.8	2.53	30M	FOLDING ENDURANCE, MIT, WITE CENTRIFUGAL FAN
GMEANS:		24.3	72.9			1.00		
		95% ELLIPSE:		39.2	16.7	WITH GAMMA = 79 DEGREES		

FOLDING ENDURANCE (MIT)

SAMPLE J29 = 24. DOUBLE FOLDS

SAMPLE J31 = 73. DOUBLE FOLDS

DOUBLE FOLDS

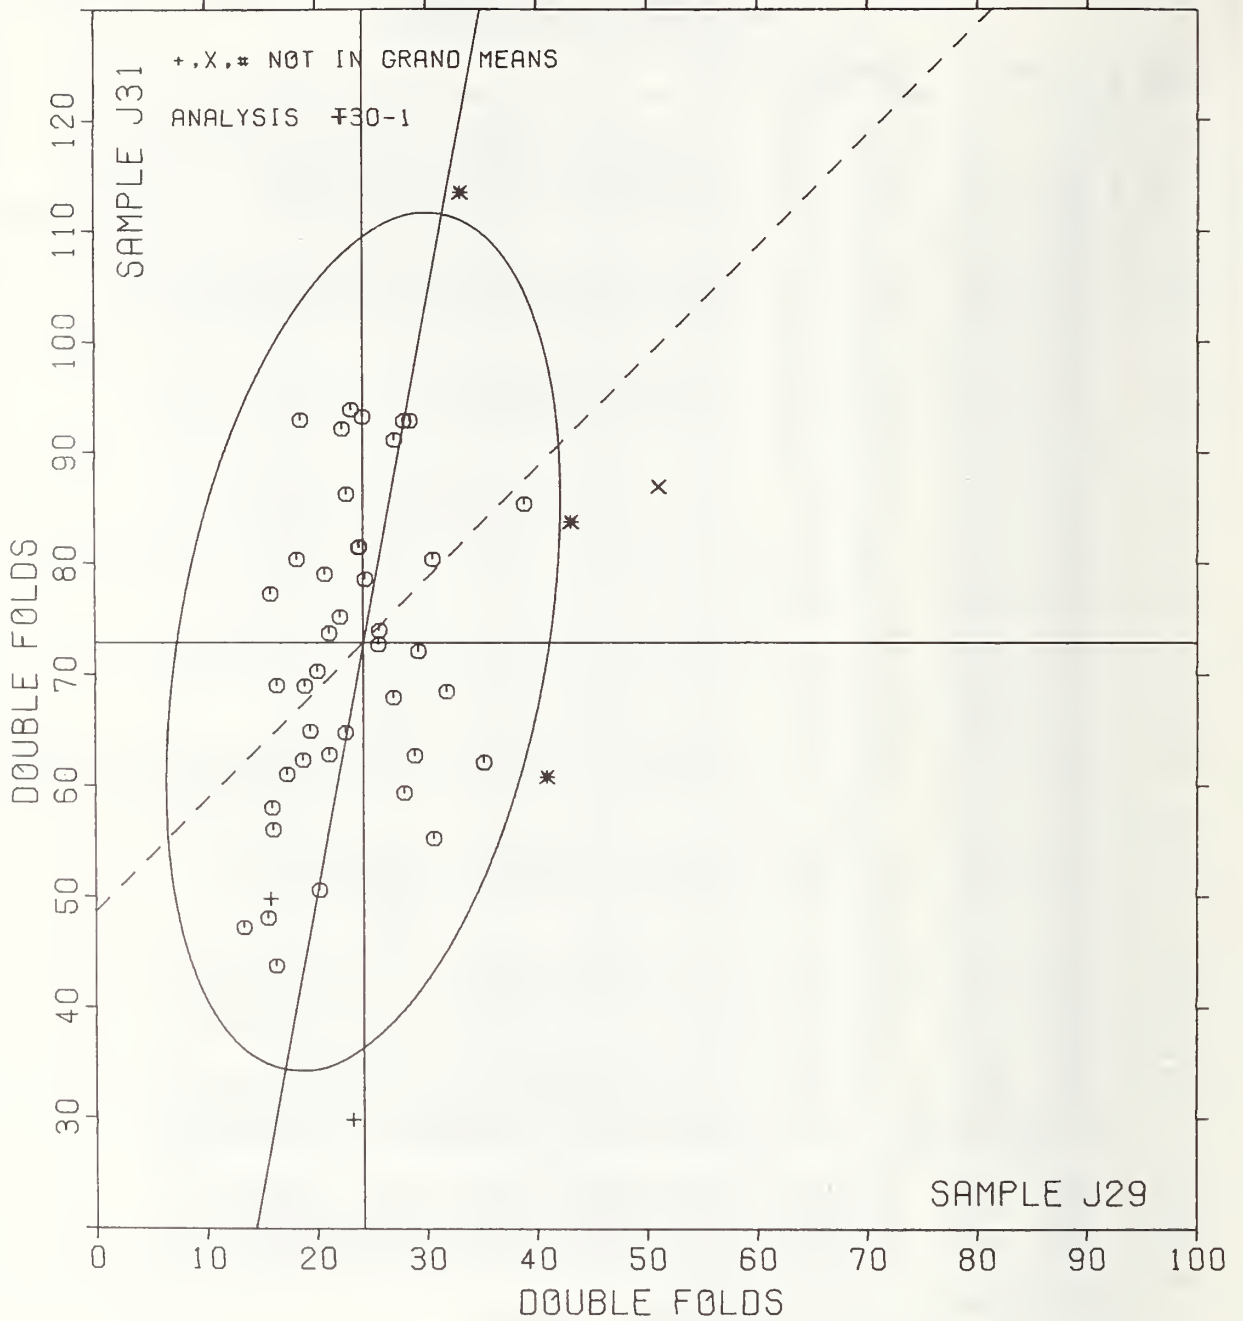

ANALYSIS T30-2 TABLE 1

FOLDING ENDURANCE (MIT)

DATA IS LOG(BASE 10) OF THE DOUBLE FOLD MEASUREMENT

LAB CODE	SAMPLE J29 MEAN	PRINTING 102 GRAMS PER SQUARE METER				SAMPLE J31 MEAN	PRINTING 86 GRAMS PER SQUARE METER				TEST D. = 15		
		DEV	N.DEV	SDR	R.SDR		DEV	N.DEV	SDR	R.SDR	VAR	F	LAB
L100M	1.202	-.141	-1.26	.110	.71	1.833	-.006	-.06	.078	.66	30M	Ø	L100M
L100N	1.196	-.147	-1.31	.066	.42	1.886	.047	.49	.044	.38	30N	Ø	L100N
L105	1.291	-.051	-.46	.207	1.33	1.873	.034	.36	.053	.45	30M	Ø	L105
L121	1.296	-.046	-.41	.264	1.70	1.888	.049	.50	.088	.75	30M	Ø	L121
L122	1.429	.087	.78	.254	1.64	1.760	-.078	-.81	.295	2.51	30M	Ø	L122
L124	1.392	.050	.45	.242	1.56	1.791	-.047	-.49	.077	.65	30N	Ø	L124
L150	1.428	.085	.76	.226	1.46	1.888	.050	.51	.128	1.09	30M	Ø	L150
L159	1.523	.181	1.62	.234	1.50	1.919	.081	.83	.107	.91	30N	Ø	L159
L162	1.307	-.036	-.32	.203	1.31	1.785	-.053	-.55	.162	1.38	30M	Ø	L162
L163	1.467	.124	1.11	.131	.84	1.718	-.121	-1.25	.152	1.30	30N	Ø	L163
L176	1.424	.082	.73	.081	.52	1.823	-.015	-.16	.091	.78	30N	Ø	L176
L182M	1.389	.047	.42	.219	1.41	1.959	.121	1.25	.088	.75	30M	Ø	L182M
L185	1.356	.014	.12	.145	.93	1.903	.064	.67	.087	.74	30N	Ø	L185
L190C	1.461	.119	1.07	.068	.44	1.847	.008	.08	.100	.85	30N	Ø	L190C
L212	1.259	-.084	-.75	.121	.78	1.788	-.051	-.52	.078	.67	30M	Ø	L212
L223F	1.303	-.040	-.35	.134	.86	1.858	.019	.20	.095	.81	30M	Ø	L223F
L230	1.270	-.072	-.64	.135	.87	1.792	-.046	-.48	.132	1.13	30N	Ø	L230
L232	1.433	.091	.82	.110	.71	1.931	.092	.95	.210	1.78	30N	Ø	L232
L236	1.246	-.096	-.86	.116	.75	1.901	.063	.65	.059	.50	30N	Ø	L236
L238A	1.309	-.033	-.30	.127	.82	1.761	-.078	-.81	.195	1.66	30N	Ø	L238A
L238B	1.183	-.159	-1.43	.145	.93	1.752	-.087	-.90	.109	.93	30D	Ø	L238B
L243	1.368	.026	.23	.123	.79	1.962	.123	1.27	.085	.73	30D	Ø	L243
L254	1.104	-.238	-2.13	.150	.96	1.662	-.177	-1.83	.105	.89	30M	Ø	L254
L262	1.286	-.056	-.50	.128	.82	1.839	.000	.00	.086	.73	30N	Ø	L262
L275	1.253	-.089	-.80	.126	.81	1.957	.118	1.22	.105	.90	30N	Ø	L275
L278	1.186	-.156	-1.40	.080	.52	1.668	-.171	-1.77	.113	.97	30C	Ø	L278
L279	1.275	-.067	-.60	.168	1.08	1.621	-.217	-2.25	.289	2.46	30N	Ø	L279
L285A	1.361	.018	.17	.129	.83	1.898	.059	.61	.123	1.05	30N	Ø	L285A
L285B	1.329	-.014	-.12	.140	.90	1.937	.098	1.01	.169	1.44	30N	Ø	L285B
L299	1.299	-.043	-.39	.135	.87	1.887	.048	.50	.107	.91	30N	Ø	L299
L320	1.519	.176	1.58	.319	2.06	1.897	.058	.60	.170	1.45	30N	Ø	L320
L326N	1.197	-.145	-1.30	.119	.77	1.620	-.219	-2.27	.138	1.18	30N	Ø	L326N
L339	1.264	-.078	-.70	.110	.71	1.832	-.007	-.07	.081	.69	30N	Ø	L339
L366A	1.395	.052	.47	.124	.80	1.847	.008	.09	.142	1.21	30N	Ø	L366A
L376	1.189	-.153	-1.37	.126	.81	1.742	-.097	-1.00	.078	.66	30N	Ø	L376
L378	1.353	.011	.10	.107	.69	1.967	.129	1.33	.070	.60	30N	Ø	L378
L388	1.348	.005	.05	.097	.63	1.932	.093	.96	.061	.52	30N	Ø	L388
L390	1.369	.027	.24	.177	1.14	1.834	-.005	-.05	.155	1.32	30N	Ø	L390
L393	1.230	-.112	-1.00	.089	.57	1.765	-.074	-.76	.142	1.21	30M	Ø	L393
L396M	1.509	.166	1.49	.106	.68	2.046	.207	2.15	.089	.76	30N	Ø	L396M
L565	1.405	.063	.56	.190	1.23	1.763	-.076	-.78	.101	.86	30N	Ø	L565
L589	1.466	.124	1.11	.268	1.73	1.789	-.050	-.52	.065	.56	30N	Ø	L589
L599	1.412	.070	.63	.141	.91	1.949	.110	1.14	.099	.84	30C	Ø	L599
L622	1.634	.292	2.61	.254	1.63	1.918	.079	.82	.150	1.28	30M	*	L622
L670	1.487	.145	1.30	.341	2.20	1.755	-.083	-.86	.166	1.41	30N	Ø	L670

GR. MEAN = 1.342 LOG(10) FOLD GRAND MEAN = 1.839 LOG(10) FOLD TEST DETERMINATIONS = 15
 SD MEANS = .112 LOG(10) FOLD SD OF MEANS = .097 LOG(10) FOLD 45 LABS IN GRAND MEANS
 AVERAGE SDR = .155 LOG(10) FOLD AVERAGE SDR = .117 LOG(10) FOLD

L182S	1.312	-.031	-.27	.251	1.61	2.154	.316	3.27	.133	1.13	30S	*	L182S
L190D	1.412	.070	.63	.120	.77	2.185	.346	3.58	.113	.97	30S	*	L190D
L280	1.185	-.157	-1.41	.113	.73	1.670	-.169	-1.74	.177	1.51	30K	*	L280
L326S	1.332	-.010	-.09	.122	.79	2.063	.224	2.32	.131	1.11	30S	*	L326S
L396S	1.362	.019	.17	.068	.44	1.464	-.374	-3.87	.101	.86	30T	*	L396S

TOTAL NUMBER OF LABORATORIES REPORTING = 50

The ISO (International Standards Organization) is proposing that MIT folding endurance be reported as the logarithm (to the base 10) of the double fold instead of the double fold as in the past.

Analysis T30-1 in this report is the same as in the past with no changes. This analysis, T30-2, shows the data as the ISO proposes. This analysis used the raw data reported for T30-1. The raw data are converted to the logarithm (base 10) as shown in the example to the right, and then the mean of the converted data is calculated and reported as ISO folding endurance.

Raw data (Folding number in double folds)	log (base 10) of raw data
207	2.32
166	2.22
151	2.18
332	2.52
260	2.41
137	2.14
199	2.30
230	2.36
210	2.31

mean of raw data


mean of logs
"Folding endurance"

FOLDING ENDURANCE (MIT)
DATA IS LOG(BASE 10) OF THE DOUBLE FOLD MEASUREMENT

LAB CODE	F	MEANS		COORDINATES		AVG R. SDR	VAR	PROPERTY	TEST	INSTRUMENT	CONDITIONS
		J29	J31	MAJOR	MINOR						
L254	Ø	1.104	1.662	-.296	-.006	.93	30M	FOLDING	ENDURANCE,	MIT,	WITE CENTRIFUGAL FAN
L238B	Ø	1.183	1.752	-.180	.022	.93	30D	FOLDING	ENDURANCE,	MIT,	MODIFIED DRIVE TO REDUCE HEATING
L280	*	1.185	1.670	-.226	-.046	1.12	30K	FOLDING	ENDURANCE,	MIT,	KÖBLER-MÖLIN
L278	Ø	1.186	1.668	-.226	-.048	.74	30C	FOLDING	ENDURANCE,	MIT,	CIRCULATING FAN IN CEILING
L376	Ø	1.189	1.742	-.181	.010	.74	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L100N	Ø	1.196	1.886	-.092	.124	.40	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L326N	Ø	1.197	1.620	-.245	-.094	.97	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L100M	Ø	1.202	1.833	-.118	.077	.69	30M	FOLDING	ENDURANCE,	MIT,	WITH CENTRIFUGAL FAN
I393	Ø	1.230	1.765	-.134	.005	.89	30M	FOLDING	ENDURANCE,	MIT,	WITH CENTRIFUGAL FAN
L236	Ø	1.246	1.901	-.042	.107	.62	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L275	Ø	1.253	1.957	-.004	.148	.85	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L212	Ø	1.259	1.788	-.098	.008	.72	30M	FOLDING	ENDURANCE,	MIT,	WITH CENTRIFUGAL FAN
L339	Ø	1.264	1.832	-.068	.040	.70	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L230	Ø	1.270	1.792	-.086	.004	1.00	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L279	Ø	1.275	1.621	-.181	-.138	1.77	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L262	Ø	1.286	1.839	-.046	.033	.78	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L105	Ø	1.291	1.873	-.022	.058	.89	30M	FOLDING	ENDURANCE,	MIT,	WITH CENTRIFUGAL FAN
L121	Ø	1.296	1.888	-.009	.066	1.22	30M	FOLDING	ENDURANCE,	MIT,	WITH CENTRIFUGAL FAN
L299	Ø	1.299	1.887	-.007	.064	.89	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L223F	Ø	1.303	1.858	-.021	.039	.84	30M	FOLDING	ENDURANCE,	MIT,	WITE CENTRIFUGAL FAN
L162	Ø	1.307	1.785	-.060	-.023	1.34	30M	FOLDING	ENDURANCE,	MIT,	WITE CENTRIFUGAL FAN
L238A	Ø	1.309	1.761	-.072	-.044	1.24	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L182S	*	1.312	2.154	.159	.275	1.37	30S	FOLDING	ENDURANCE,	MIT,	SCHÖPPER, LEIPZIG
L285B	Ø	1.329	1.937	.046	.088	1.17	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L326S	*	1.332	2.063	.122	.188	.95	30S	FOLDING	ENDURANCE,	MIT,	SCHÖPPER, LEIPZIG
L388	Ø	1.348	1.932	.058	.073	.57	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L378	Ø	1.353	1.967	.084	.098	.64	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L185	Ø	1.356	1.903	.049	.044	.84	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L285A	Ø	1.362	1.898	.049	.037	.94	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L396S	*	1.362	1.464	-.202	-.316	.65	30T	FOLDING	ENDURANCE,	MIT,	SCHÖPPER, TMI
L243	Ø	1.368	1.962	.092	.085	.76	30D	FOLDING	ENDURANCE,	MIT,	MODIFIED DRIVE TO REDUCE HEATING
L390	Ø	1.369	1.834	.019	-.019	1.23	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L182M	Ø	1.389	1.959	.108	.071	1.08	30M	FOLDING	ENDURANCE,	MIT,	WITE CENTRIFUGAL FAN
L124	Ø	1.392	1.791	.013	-.068	1.10	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L366A	Ø	1.395	1.847	.048	-.024	1.00	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L555	Ø	1.405	1.763	.007	-.098	1.04	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L599	Ø	1.412	1.949	.121	.049	.87	30C	FOLDING	ENDURANCE,	MIT,	CIRCULATING FAN IN CEILING
L190D	*	1.412	2.185	.258	.241	.87	30S	FOLDING	ENDURANCE,	MIT,	SCHÖPPER, LEIPZIG
L176	Ø	1.424	1.823	.058	-.060	.65	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L150	Ø	1.428	1.888	.058	-.009	1.27	30M	FOLDING	ENDURANCE,	MIT,	WITE CENTRIFUGAL FAN
L122	Ø	1.429	1.760	.025	-.114	2.07	30M	FOLDING	ENDURANCE,	MIT,	WITH CENTRIFUGAL FAN
L232	Ø	1.433	1.931	.128	.022	1.25	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L190C	Ø	1.461	1.847	.101	-.063	.64	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L589	Ø	1.466	1.789	.072	-.112	1.14	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L163	Ø	1.467	1.718	.031	-.171	1.07	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L670	Ø	1.487	1.755	.070	-.152	1.81	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L396M	Ø	1.509	2.046	.256	.072	.72	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L320	Ø	1.519	1.897	.177	-.055	1.75	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L159	Ø	1.523	1.919	.194	-.040	1.21	30N	FOLDING	ENDURANCE,	MIT,	NO CENTRIFUGAL FAN
L622	*	1.634	1.918	.283	-.105	1.46	30M	FOLDING	ENDURANCE,	MIT,	WITH CENTRIFUGAL FAN
GMEANS:		1.342	1.839			1.00					
		95% BLLIPSE:		.322	.200						WITE GAMMA * 35 DEGREES

FOLDING ENDURANCE (MIT)

SAMPLE J29 = 1.34 LOG(10) FOLD SAMPLE J31 = 1.84 LOG(10) FOLD

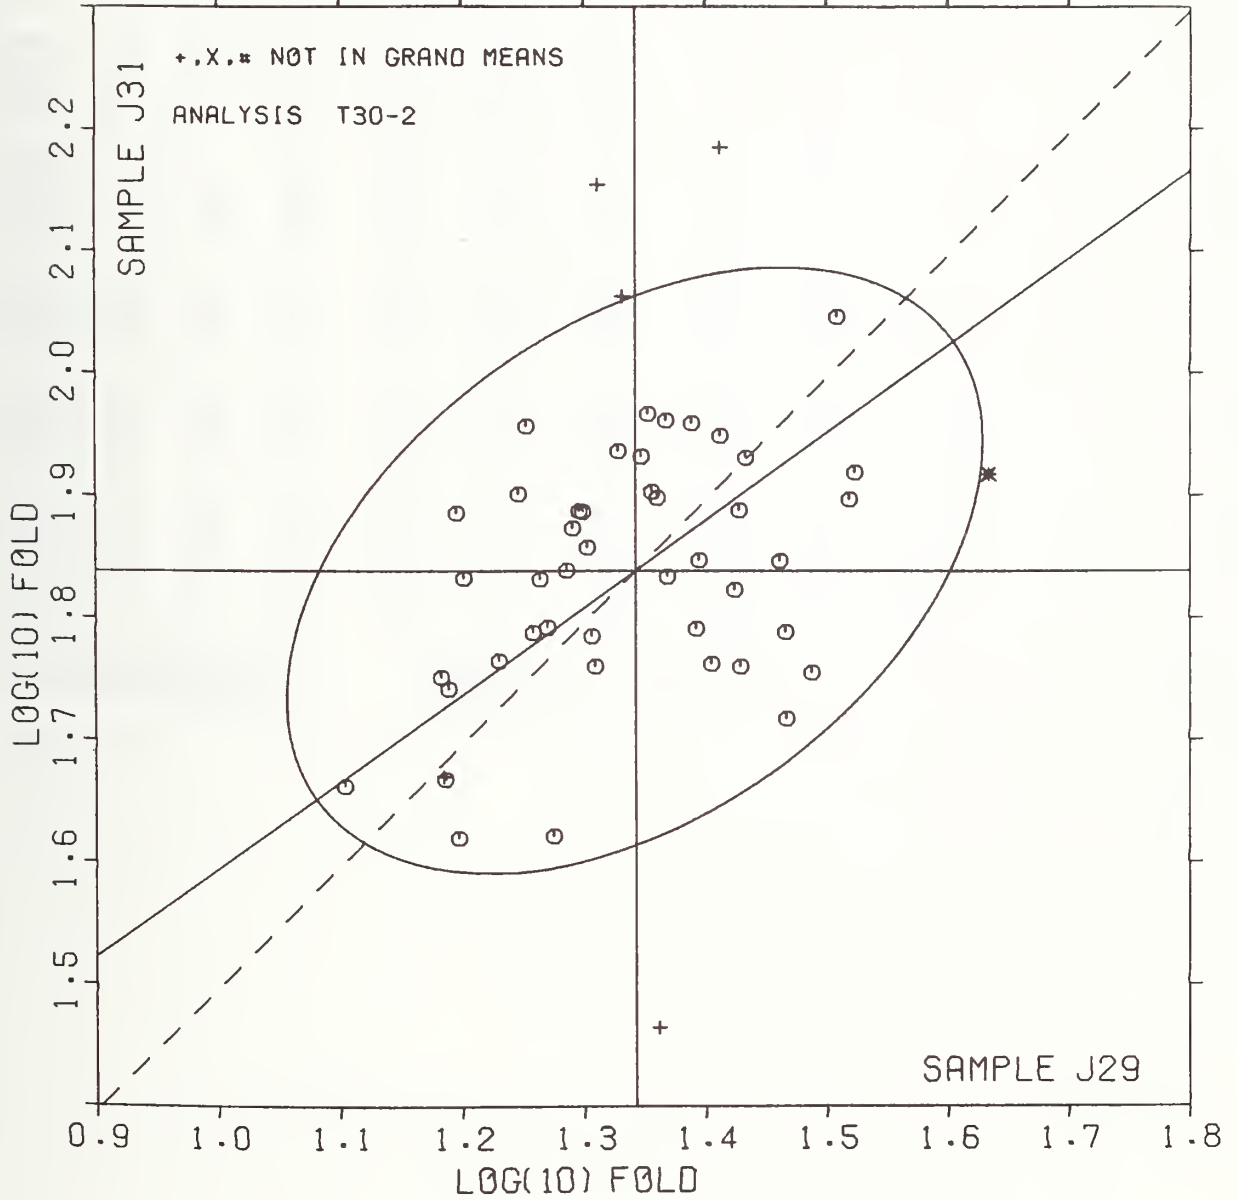

RESULTS EXPRESSED IN STANDARD GURLEY UNITS; MILLIGRAMS PER A 1X3 INCH SPECIMEN (ACTUAL LENGTH 3.5 INCHES)

LAB CODE	SAMPLE H69 MEAN	PRINTING 96 GRAMS PER SQUARE METER				SAMPLE J25 MEAN	PRINTING 103 GRAMS PER SQUARE METER				TEST D. = 10		
		DEV	N. DEV	SDR	R. SDR		DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L100	445.	-7.	-.24	15.	.71	244.	3.	.17	10.	.72	350	Ø	L100
L121	498.	46.	1.68	15.	.71	268.	26.	1.57	15.	1.09	350	Ø	L121
L132	396.	-56.	-2.01	25.	1.18	236.	-6.	-.34	8.	.63	350	*	L132
L139	442.	-10.	-.35	12.	.60	250.	8.	.48	17.	1.26	350	Ø	L139
L148	445.	-6.	-.22	16.	.78	236.	-5.	-.32	15.	1.14	350	Ø	L148
L159	437.	-15.	-.53	19.	.93	229.	-13.	-.77	16.	1.15	350	Ø	L159
L162	5.	-447.	-16.14	0.	.01	5.	-237.	-14.13	0.	.02	350	#	L162
L163	442.	-10.	-.34	37.	1.78	227.	-14.	-.85	23.	1.68	350	Ø	L163
L183	517.	66.	2.38	31.	1.50	268.	26.	1.55	16.	1.17	350	Ø	L183
L190C	394.	-57.	-2.07	15.	.74	195.	-47.	-2.78	12.	.91	350	*	L190C
L195	493.	42.	1.50	36.	1.75	276.	34.	2.03	13.	.99	350	Ø	L195
L212	448.	-3.	-.11	30.	1.44	252.	10.	.60	10.	.71	350	Ø	L212
L223	433.	-18.	-.66	15.	.71	230.	-11.	-.67	8.	.62	350	Ø	L223
L224	470.	19.	.67	17.	.79	252.	10.	.59	18.	1.37	350	Ø	L224
L232	473.	21.	.76	19.	.90	235.	-6.	-.38	12.	.89	350	Ø	L232
L236	415.	-36.	-1.30	28.	1.36	207.	-34.	-2.06	11.	.82	350	Ø	L236
L249	458.	7.	.24	28.	1.34	249.	8.	.47	14.	1.04	350	Ø	L249
L254	411.	-41.	-1.46	15.	.70	222.	-20.	-1.19	6.	.46	350	Ø	L254
L260	444.	-8.	-.27	14.	.67	244.	2.	.11	5.	.38	350	Ø	L260
L285	435.	-16.	-.58	23.	1.12	261.	20.	1.18	11.	.83	350	Ø	L285
L291	463.	12.	.42	19.	.93	246.	4.	.23	23.	1.67	350	Ø	L291
L308	461.	9.	.33	35.	1.67	237.	-4.	-.27	14.	1.02	350	Ø	L308
L356	442.	-8.	-.30	22.	1.06	226.	-16.	-.96	8.	.57	350	Ø	L356
L376	469.	17.	.61	18.	.85	245.	3.	.20	23.	1.72	350	Ø	L376
L378	443.	-9.	-.31	18.	.85	237.	-5.	-.28	25.	1.85	350	Ø	L378
L382	467.	15.	.55	21.	.99	247.	5.	.30	13.	.98	350	Ø	L382
L390	460.	8.	.29	27.	1.30	242.	0.	.01	9.	.68	350	Ø	L390
L396	445.	-7.	-.24	15.	.70	248.	7.	.40	9.	.69	350	Ø	L396
L600	465.	13.	.48	12.	.57	245.	4.	.21	8.	.56	350	Ø	L600
L648	489.	38.	1.37	13.	.60	252.	11.	.64	6.	.43	350	Ø	L648
L650	443.	-9.	-.31	14.	.68	244.	2.	.11	20.	1.50	350	Ø	L650

GR. MEAN = 452. GURLEY UNITS GRAND MEAN = 242. GURLEY UNITS TEST DETERMINATIONS = 10
SD MEANS = 28. GURLEY UNITS SD OF MEANS = 17. GURLEY UNITS 30 LABS IN GRAND MEANS
AVERAGE SDR = 21. GURLEY UNITS AVERAGE SDR = 13. GURLEY UNITS

L213 477. 26. .94 31. 1.51 235. -7. -.41 9. .67 350 * L213
TOTAL NUMBER OF LABORATORIES REPORTING = 32

Best values: H69 450 ± 50 Gurley units
J25 240 ± 30 Gurley units


Data from the following laboratories appear to be off by a multiplicative factor: 162

RESULTS EXPRESSED IN STANDARD GURLEY UNITS: MILLIGRAMS FOR A 1X3 INCH SPECIMEN (ACTUAL LENGTH 3.5 INCHES)

LAB CODE	P	MEANS		COORDINATES		AVG		PROPERTY	TEST INSTRUMENT	CONDITIONS
		H69	J25	MAJOR	MINOR	R.SDR	VAR			
L162	#	5.	5.	-506.	-1.	.01	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L190C	*	394.	195.	-72.	-14.	.83	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L132	*	396.	236.	-52.	21.	.90	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L254	Ø	411.	222.	-45.	1.	.58	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L236	Ø	415.	207.	-48.	-14.	1.09	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L223	Ø	433.	230.	-21.	-2.	.66	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L285	Ø	435.	261.	-5.	25.	.97	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L159	Ø	437.	229.	-19.	-5.	1.04	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L139	Ø	442.	250.	-5.	12.	.93	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L163	Ø	442.	227.	-15.	-8.	1.73	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L650	Ø	443.	244.	-7.	6.	1.09	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L378	Ø	443.	237.	-10.	-0.	1.35	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L356	Ø	443.	226.	-15.	-10.	.81	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L260	Ø	444.	244.	-6.	5.	.52	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L396	Ø	445.	248.	-3.	9.	.69	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L100	Ø	445.	244.	-4.	6.	.71	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L148	Ø	445.	236.	-8.	-2.	.96	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L212	Ø	448.	252.	2.	10.	1.08	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L249	Ø	458.	249.	10.	4.	1.19	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L390	Ø	460.	242.	7.	-4.	.99	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L308	Ø	461.	237.	6.	-8.	1.35	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L291	Ø	463.	246.	12.	-2.	1.30	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L600	Ø	465.	245.	13.	-3.	.57	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L382	Ø	467.	247.	16.	-3.	.99	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L376	Ø	465.	245.	17.	-5.	1.29	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L224	Ø	470.	252.	21.	0.	1.08	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L232	Ø	473.	235.	16.	-15.	.90	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L213	*	477.	235.	20.	-18.	1.09	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	TEST PIECE), 20 C, 65% RH
L648	Ø	480.	252.	39.	-8.	.52	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L195	Ø	492.	276.	53.	11.	1.37	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L121	Ø	498.	268.	53.	2.	.90	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
L183	Ø	517.	268.	70.	-8.	1.34	350	STIFFNESS,	GURLEY (UNITS: MG/1X3	-ACTUALLY 3.5= TEST PIECE)
GMEANS:		452.	242.			1.00				
		95% ELLIPSE:		81.	25.			WITH GAMMA = 27 DEGREES		

STIFFNESS, GURLEY

SAMPLE H69 = 452. GURLEY UNITS SAMPLE J25 = 242. GURLEY UNITS

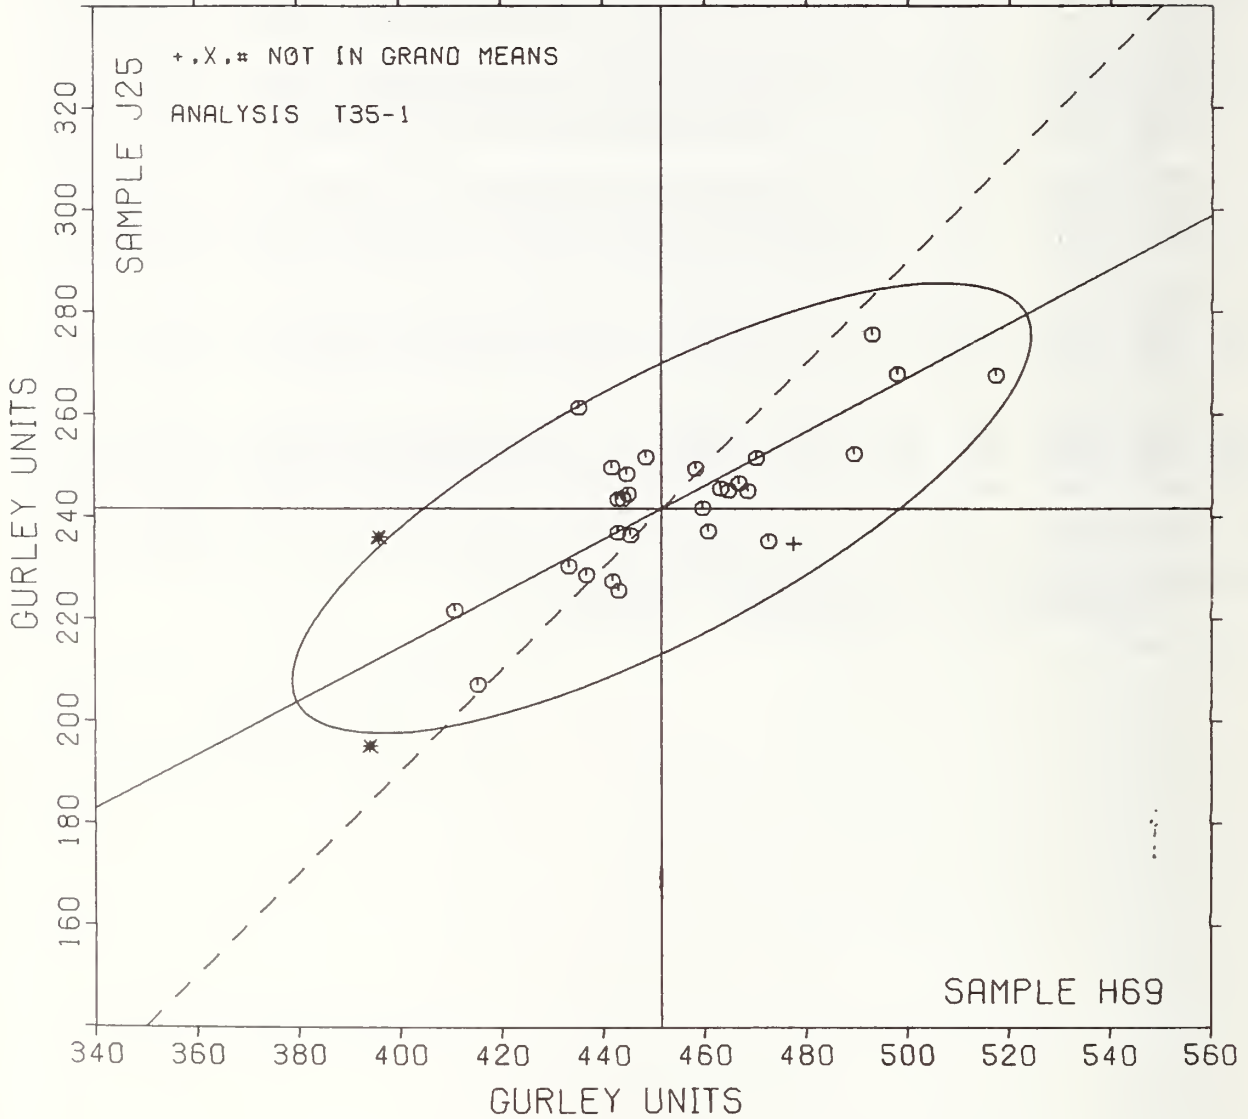

ANALYSIS T36-1 TABLE 1

TABER STIFFNESS

TAPPI STANDARD T489 09-76, RESULTS EXPRESSED IN GRAM CENTIMETERS

LAB CODE	SAMPLE J10 MEAN	PRINTING 149 GRAMS PER SQUARE METER				SAMPLE J69 MEAN	PRINTING 149 GRAMS PER SQUARE METER				TEST D. = 10		
		DEV	N. DEV	SDR	R. SDR		DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L107A	16.63	.11	.10	1.18	1.56	6.52	.56	.55	.17	.49	36T	Ø	L107A
L122	15.76	-.76	-.75	.54	.72	6.34	.38	.37	.42	1.22	36T	Ø	L122
L123	16.20	-.32	-.32	2.04	2.71	6.80	.84	.82	.63	1.83	36T	Ø	L123
L126	15.65	-.67	-.86	.32	.42	4.50	-1.46	-1.43	.18	.53	36T	Ø	L126
L150	16.70	.18	.17	.82	1.09	6.60	.64	.63	.52	1.50	36T	Ø	L150
L163	17.00	.48	.47	.41	.54	5.43	-.52	-.51	.30	.88	36T	Ø	L163
L1738	15.40	-1.12	-1.10	.52	.68	6.20	.24	.24	.42	1.22	36T	Ø	L1738
L176	17.10	.58	.57	.39	.52	5.04	-.92	-.90	.13	.37	36T	Ø	L176
L182	17.22	.70	.68	.75	.99	6.16	.20	.20	.26	.76	36T	Ø	L182
L207	16.89	.37	.36	.57	.75	6.93	.97	.95	.44	1.29	36T	Ø	L207
L212	14.85	-1.67	-1.64	.53	.70	4.95	-1.01	-.99	.14	.42	36T	Ø	L212
L228	17.30	.78	.76	1.34	1.77	10.60	4.64	4.54	.84	2.44	36T	#	L228
L230	18.20	1.68	1.65	2.20	2.91	6.00	.04	.04	.82	2.36	36T	Ø	L230
L236	51.00	34.48	33.88	2.67	3.53	21.40	15.44	15.11	1.17	3.40	36T	#	L236
L242	16.35	-.17	-.17	.65	.86	6.30	.34	.34	.20	.57	36T	Ø	L242
L243	16.85	.33	.32	.88	1.17	8.05	2.09	2.05	.13	.37	36T	Ø	L243
L260	16.67	.15	.15	.35	.47	5.92	-.03	-.03	.17	.49	36T	Ø	L260
L262	17.90	1.38	1.35	1.05	1.39	6.50	.94	.92	.21	.61	36T	Ø	L262
L281	17.12	.60	.59	.34	.45	4.87	-1.08	-1.06	.25	.72	36T	Ø	L281
L318	15.62	-.90	-.88	.49	.65	6.12	.17	.16	.21	.62	36T	Ø	L318
L324	17.45	.93	.91	.50	.66	4.85	-1.10	-1.07	.14	.41	36T	Ø	L324
L339	15.18	-1.34	-1.32	.38	.51	3.98	-1.98	-1.94	.59	1.70	36T	Ø	L339
L388	27.45	10.93	10.74	3.13	4.15	15.70	9.74	9.53	1.69	4.88	36T	#	L388
L442	16.56	.04	.04	1.26	1.67	6.77	.81	.80	1.07	3.10	36T	Ø	L442
L484	13.58	-2.54	-2.50	.64	.85	3.88	-2.08	-2.03	.19	.56	36T	Ø	L484
L570	18.00	1.48	1.45	.67	.88	7.00	1.04	1.02	.00	.00	36T	Ø	L570
L580	17.40	.88	.86	.70	.93	6.40	.44	.43	.52	1.50	36T	Ø	L580
L616	22.00	5.48	5.38	2.49	3.30	5.80	-.16	-.15	.79	2.29	36T	#	L616
L651	16.40	-.12	-.12	.70	.93	6.40	.44	.43	.52	1.50	36T	Ø	L651

GR. MEAN = 16.52 TABER UNITS GRAND MEAN = 5.96 TABER UNITS TEST DETERMINATIONS = 10
 SD MEANS = 1.02 TABER UNITS SD OF MEANS = 1.02 TABER UNITS 25 LABS IN GRAND MEANS
 AVERAGE SDR = .76 TABER UNITS AVERAGE SDR = .35 TABER UNITS

TOTAL NUMBER OF LABORATORIES REPORTING = 29

Best values: J10 16.6 ± 1.5 Taber units
 J69 6.1 ± 1.6 Taber units

The following laboratories were omitted from the grand means because of extreme test results: 228, 388, 616


Data from the following laboratories appear to be off by a multiplicative factor: 236

TAPPI STANDARD T489 OS-76, RESULTS EXPRESSED IN GRAM CENTIMETERS

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---CONDITIONS
		J10	J69	MAJOR	MINOR	R.SDR	VAR	
L484	Ø	13.98	3.88	-3.27	.34	.70	36T	STIFFNESS, TABER
L212	Ø	14.85	4.95	-1.89	.48	.56	36T	STIFFNESS, TABER
L339	Ø	15.18	3.98	-2.35	-.44	1.10	36T	STIFFNESS, TABER
L173B	Ø	15.40	6.20	-.62	.97	.95	36T	STIFFNESS, TABER
L37.8	Ø	15.62	6.12	-.51	.76	.63	36T	STIFFNESS, TABER
L126	Ø	15.65	4.50	-1.65	-.41	.48	36T	STIFFNESS, TABER
L122	Ø	15.76	6.34	-.26	.81	.97	36T	STIFFNESS, TABER
L123	Ø	16.20	6.80	.37	.82	2.27	36T	STIFFNESS, TABER
L242	Ø	16.35	6.30	.12	.36	.71	36T	STIFFNESS, TABER
L651	Ø	16.40	6.40	.23	.40	1.21	36T	STIFFNESS, TABER
L442	Ø	16.56	6.77	.60	.55	2.38	36T	STIFFNESS, TABER
L107A	Ø	16.63	6.52	.47	.32	1.02	36T	STIFFNESS, TABER
L260	Ø	16.67	5.92	.08	-.13	.48	36T	STIFFNESS, TABER
L150	Ø	16.70	6.60	.58	.33	1.29	36T	STIFFNESS, TABER
L243	Ø	16.85	8.05	1.72	1.24	.77	36T	STIFFNESS, TABER
L207	Ø	16.89	6.93	.95	.42	1.02	36T	STIFFNESS, TABER
L163	Ø	17.00	5.43	-.04	-.71	.71	36T	STIFFNESS, TABER
L176	Ø	17.10	5.04	-.25	-1.05	.44	36T	STIFFNESS, TABER
L281	Ø	17.12	4.87	-.35	-1.19	.58	36T	STIFFNESS, TABER
L182	Ø	17.22	6.16	.63	-.35	.88	36T	STIFFNESS, TABER
L228	#	17.30	10.60	3.84	2.72	2.11	36T	STIFFNESS, TABER
L580	Ø	17.40	6.40	.93	-.31	1.21	36T	STIFFNESS, TABER
L324	Ø	17.45	4.86	-.13	-1.43	.54	36T	STIFFNESS, TABER
L262	Ø	17.90	6.90	1.64	-.31	1.00	36T	STIFFNESS, TABER
L570	Ø	18.00	7.00	1.78	-.31	.44	36T	STIFFNESS, TABER
L230	Ø	18.20	6.00	1.21	-1.16	2.64	36T	STIFFNESS, TABER
L616	#	22.00	5.80	3.74	-4.00	2.79	36T	STIFFNESS, TABER
L388	#	27.45	15.70	14.61	-.90	4.51	36T	STIFFNESS, TABER
L236	#	51.00	21.40	35.24	-13.61	3.46	36T	STIFFNESS, TABER
GMEANS:		16.52	5.96			1.00		
		95% ELLIPSE:	3.32	1.96		WITH GAMMA = 45 DEGREES		

STIFFNESS, TABER

SAMPLE J10 = 16.5 TABER UNITS SAMPLE J69 = 6.0 TABER UNITS

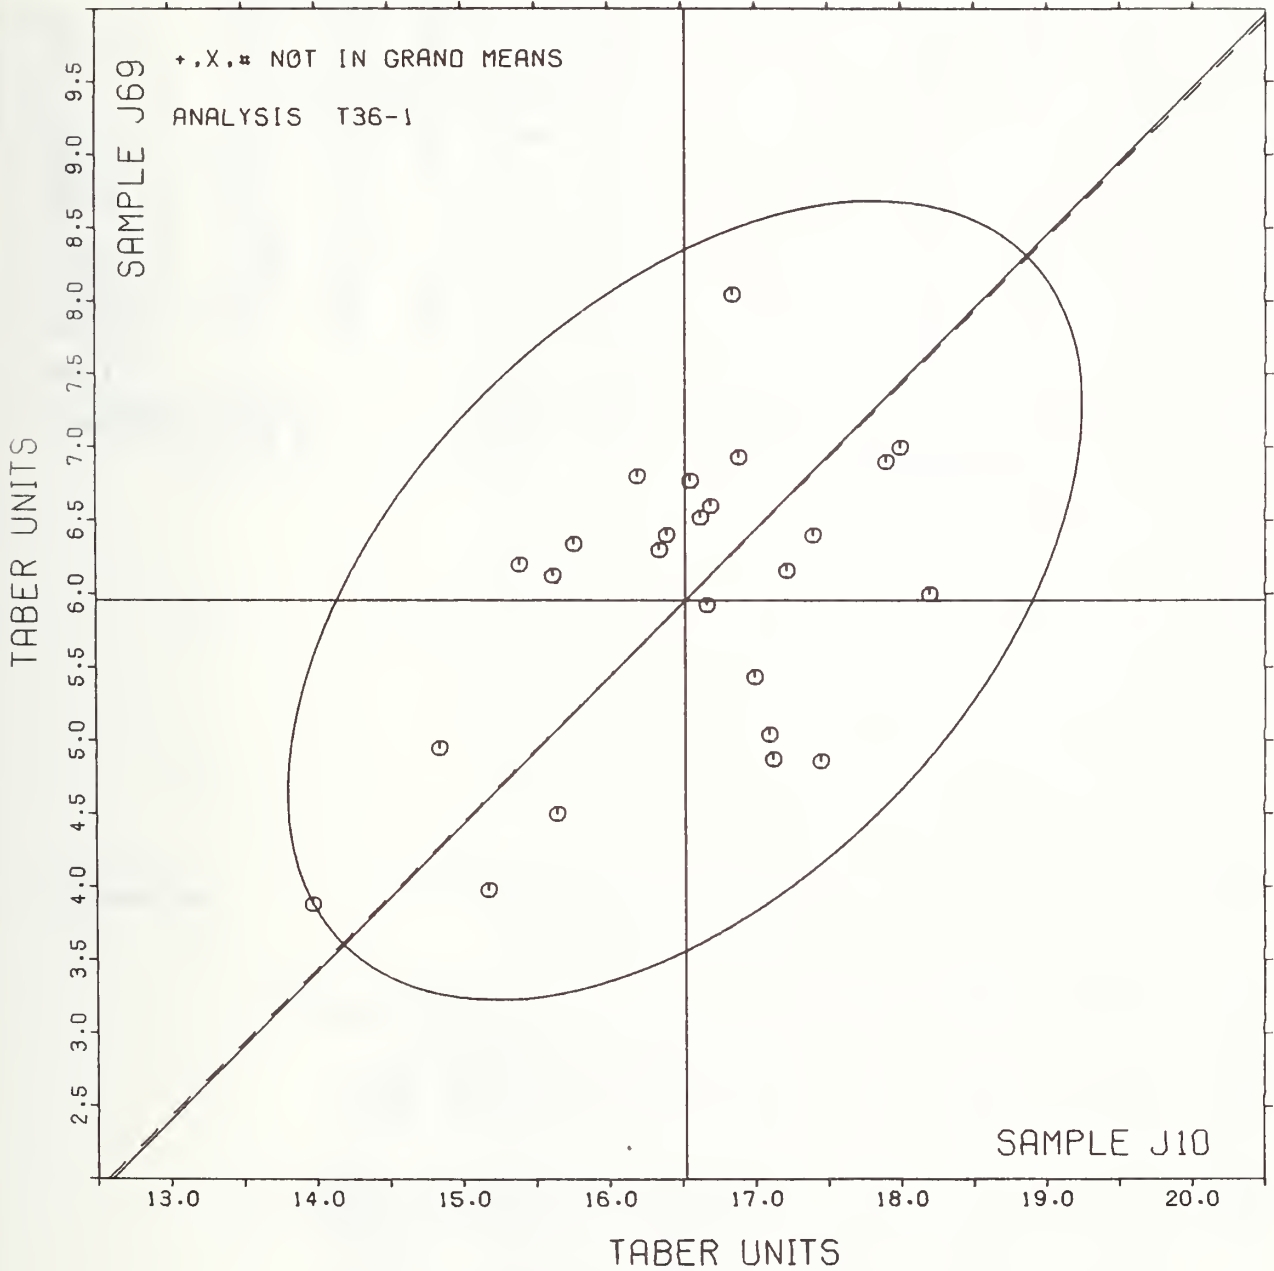

LAB CODE	SAMPLE H79		PRINTING 151 GRAMS PER SQUARE METER				SAMPLE E60		PRINTING 68 GRAMS PER SQUARE METER				TEST D. " 4		
	MEAN	DEV	N.DEV	SDR	R.SDR	MEAN	DEV	N.DEV	SDR	R.SDR	VAR	F	LAB		
L122	49.8	=36.9	=.72	2.0	.39	40.5	=34.5	=.71	2.0	.41	49Q	#	L122		
L149	68.6	=18.1	=.35	6.6	1.33	61.9	=13.6	=.28	4.8	.98	49L	#	L149		
L182I	26.1	=60.6	=1.18	.6	.11	17.5	=57.9	=1.18	.7	.15	49S	#	L182I		
L190C	56.3	=30.4	=.59	2.1	.41	45.2	=30.2	=.62	2.8	.57	49T	#	L190C		
L207	92.0	5.3	.10	4.3	.86	NO DATA REPORTED FOR SAMPLE E60						49I	#	L207	
L242	50.7	=36.0	=.70	5.5	1.10	38.5	=37.0	=.75	4.0	.83	49P	#	L242		
L243	103.2	16.6	.32	8.3	1.65	81.5	6.0	.12	7.1	1.47	49U	#	L243		
L280	3.7	=83.0	=1.61	.0	.00	3.7	=71.8	=1.47	.0	.00	49V	#	L280		
L291	88.7	2.0	.04	4.3	.86	59.5	=15.9	=.33	2.9	.60	49I	#	L291		
L388	118.8	32.1	.62	8.8	1.76	140.4	64.9	1.33	8.8	1.81	49Q	#	L388		
L484	1460.0	1373.3	26.69	40.0	8.00	1135.0	1059.5	21.63	86.6	17.80	49P	#	L484		
L564	42.8	=43.9	=.85	3.2	.65	45.6	=29.9	=.61	4.6	.94	49D	#	L564		
L598	187.2	100.5	1.95	7.8	1.56	165.9	90.5	1.85	10.7	2.20	49P	#	L598		
L616	182.5	95.8	1.86	11.9	2.38	202.5	127.0	2.59	8.7	1.78	49M	#	L616		
L643	161.2	74.6	1.45	5.8	1.17	133.5	58.0	1.18	5.1	1.04	49I	#	L643		
L651	400.0	313.3	6.09	.0	.00	400.0	324.5	6.63	.0	.00	49F	#	L651		
GR. MEAN = 86.7 KP CM/SEC			GRAND MEAN = 75.5 KP CM/SEC			TEST DETERMINATIONS = 4									
SD MPANS = 51.5 KP CM/SEC			SD OF MEANS = 49.0 KP CM/SEC			11 LABS IN GRAND MEANS									
AVERAGE SDR = 5.0 KP CM/SEC			AVERAGE SDR = 4.9 KP CM/SEC												
TOTAL NUMBER OF LABORATORIES REPORTING = 16															

Data from the following laboratories were omitted from the grand means because no viscosity values were reported: 484, 616, 651

Data from the following laboratories were omitted from the grand means because the values were outside the range of the instrument: 280

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY	TEST INSTRUMENT	CONDITIONS
		H79	E60	MAJOR	MINOR	R.SDR	VAR			
L280	#	3.7	3.7	=109.6	5.1	.00	49U	SURFACE PICK STRENGTH, IGT,	OIL	
L182I	#	26.1	17.5	=83.8	=.3	.13	49Q	SURFACE PICK STRENGTH, IGT,	IGT OIL	
L564	#	42.8	45.6	=52.4	8.6	.75	49D	SURFACE PICK STRENGTH, IGT,	INK	
L122	#	49.8	40.5	=50.8	.1	.40	49Q	SURFACE PICK STRENGTH, IGT,	IGT OIL	
L242	#	50.7	38.5	=51.5	=2.0	.96	49P	SURFACE PICK STRENGTH, IGT,	IGT OIL	
L190C	#	56.3	45.2	=42.9	=1.0	.45	49T	SURFACE PICK STRENGTH, IGT,	IPC FLUID	
L149	#	68.6	61.9	=22.5	2.6	1.15	49L	SURFACE PICK STRENGTH, IGT,	P18 FLUID	
L291	#	88.7	59.5	=9.5	=13.0	.73	49I	SURFACE PICK STRENGTH, IGT,	P18 FLUID	
L207	#	92.0				.86	49I	SURFACE PICK STRENGTH, IGT,	P18 FLUID	
L243	#	103.2	81.5	16.2	=7.0	1.56	49T	SURFACE PICK STRENGTH, IGT,	IPC FLUID	
L388	#	118.8	140.4	68.0	25.0	1.79	49Q	SURFACE PICK STRENGTH, IGT,	IGT OIL	
L643	#	161.2	133.5	94.0	=9.3	1.11	49I	SURFACE PICK STRENGTH, IGT,	P18 FLUID	
L616	#	182.5	202.5	157.0	26.1	2.08	49M	SURFACE PICK STRENGTH, IGT,	P18 FLUID	
L598	#	187.2	165.9	135.2	=3.6	1.88	49P	SURFACE PICK STRENGTH, IGT,	IGT OIL	
L651	#	400.0	400.0	450.7	19.5	.00	49F	SURFACE PICK STRENGTH, IGT,	INK	
L484	#	1460.0	1135.0	1725.4	=177.6	12.90	49P	SURFACE PICK STRENGTH, IGT,	IGT OIL	
GMEANS:		86.7	75.5			1.00				
		95% ELLIPSE:		216.3	31.1	WITH GAMMA = 43 DEGREES				


SURFACE PICK STRENGTH. IGT

SAMPLE H79 = 87.

KP CM/SEC

SAMPLE E60 = 75.

KP CM/SEC

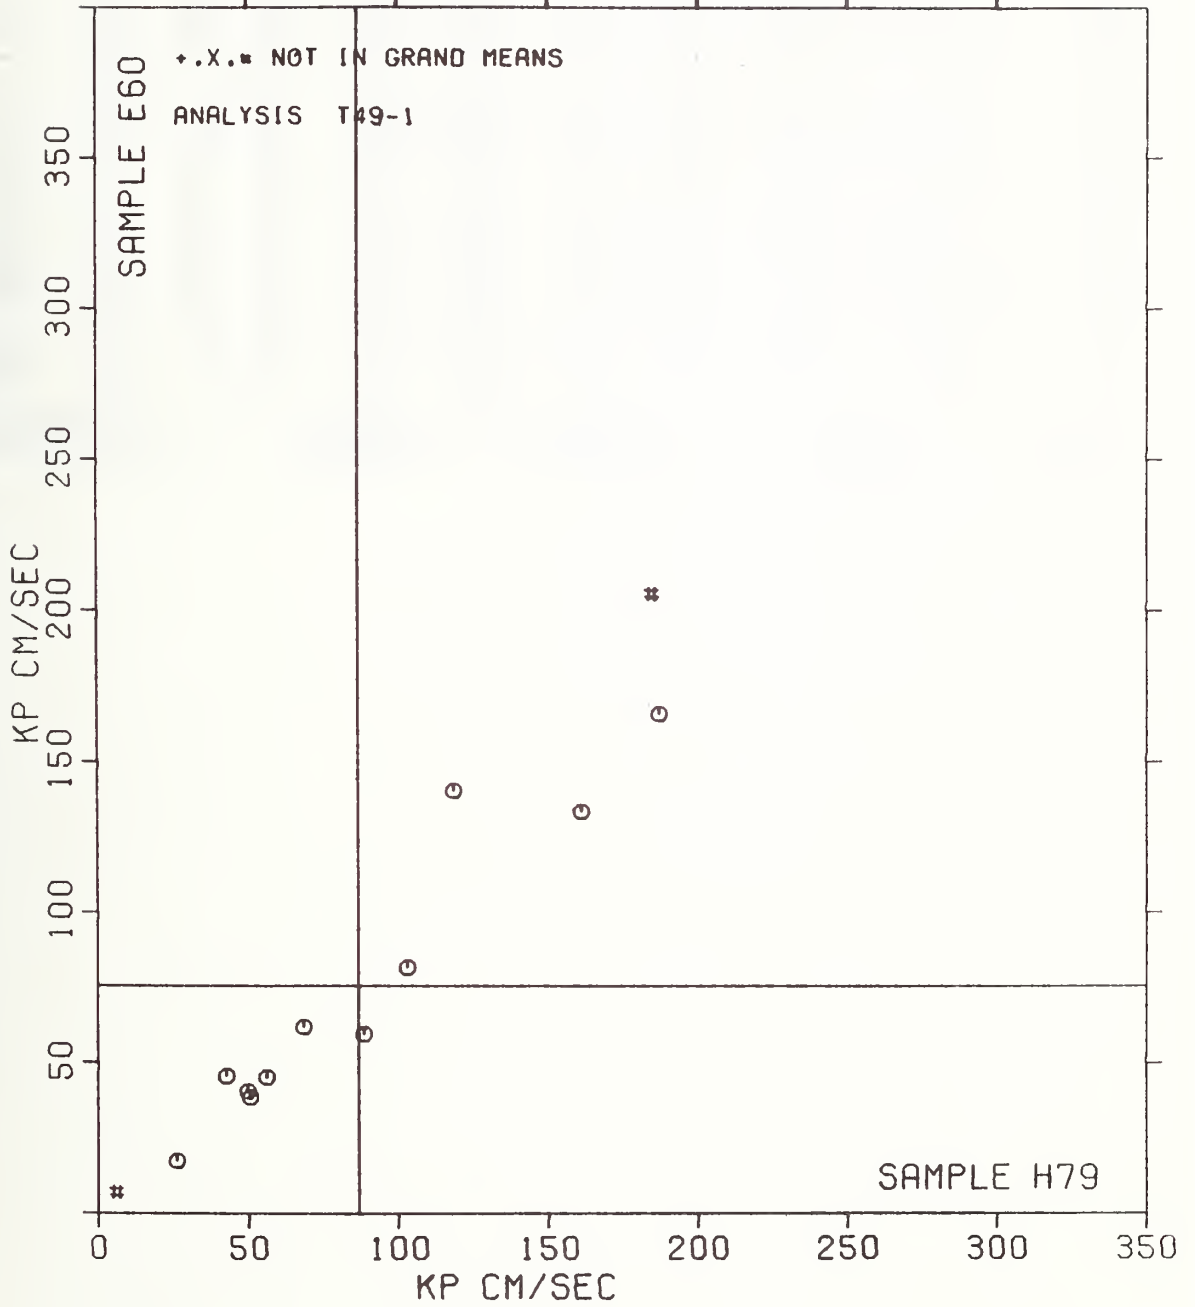

ANALYSIS T50-1 TABLE 1
 SURFACE PICK STRENGTH, WAX NUMBER
 TAPPI STANDARD T459 69-75, SURFACE STRENGTH OF PAPER (WAX PICK TEST)

LAB CODE	SAMPLE H79 MEAN	PRINTING 151 GRAMS PER SQUARE METER				R. SDR	SAMPLE J51 MEAN	PRINTING 89 GRAMS PER SQUARE METER				TEST D. 5		
		DEV	N. DEV	SDR	R. SDR			DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L105	10.40	.71	.94	.55	1.15	9.40	.45	.47	.55	1.21	50W	0	L105	
L122	9.00	-.69	-.93	.00	.00	8.20	-.75	-.78	1.10	2.41	50W	0	L122	
L162	11.00	1.31	1.74	.00	.00	9.00	.05	.05	.00	.00	50W	0	L162	
L173A	8.40	-1.29	-1.73	.55	1.15	7.20	-1.75	-1.82	.45	.99	50W	0	L173A	
L182W	10.20	.51	.68	1.10	2.29	8.60	-.35	-.37	.55	1.21	50W	0	L182W	
L183	9.80	.11	.14	.45	.94	9.00	.05	.05	.00	.00	50W	0	L183	
L195	9.20	-.49	-.66	.45	.94	9.20	.25	.26	.45	.99	50W	0	L195	
L213	10.20	.51	.68	.45	.94	10.00	1.05	1.09	.00	.00	50W	0	L213	
L225	10.40	.31	.41	.71	1.48	9.40	.45	.47	.55	1.21	50W	0	L225	
L228	10.00	.31	.41	.00	.00	7.00	-1.95	-2.03	.00	.00	50W	0	L228	
L230	9.00	-.69	-.93	.00	.00	9.20	.25	.26	.84	1.84	50W	0	L230	
L236	10.20	.51	.68	.45	.94	9.40	.45	.47	.55	1.21	50W	0	L236	
L243	8.40	-1.29	-1.73	.55	1.15	8.60	-.35	-.37	.55	1.21	50W	0	L243	
L285	10.20	.51	.68	1.10	2.29	9.40	.45	.47	.55	1.21	50W	0	L285	
L339	9.20	-.49	-.66	.45	.94	8.00	-.95	-.99	.71	1.56	50W	0	L339	
L366	9.20	-.49	-.66	.45	.94	9.80	.85	.88	.45	.99	50W	0	L366	
L378	10.40	.71	.94	.89	1.87	10.80	1.85	1.92	.45	.99	50W	0	L378	
L616	11.20	1.51	2.01	1.30	2.73	13.60	4.65	4.84	.55	1.21	50W	0	L616	

GR. MEAN = 9.69 WAX NUMBER GRAND MEAN = 8.95 WAX NUMBER TEST DETERMINATIONS = 5
 SD MEANS = .75 WAX NUMBER SD OF MEANS = .96 WAX NUMBER 17 LABS IN GRAND MEANS
 AVERAGE SDR = .48 WAX NUMBER AVERAGE SDR = .45 WAX NUMBER
 TOTAL NUMBER OF LABORATORIES REPORTING = 18

Best values: H79 9.8 ± 1.3 wax number
 J51 9.0 ± 1.7 wax number

The following laboratories were omitted from the grand means because of extreme test results: 616

ANALYSIS T80-1 TABLE 2
 SURFACE PICK STRENGTH, WAX NUMBER
 TAPPI STANDARD T489 68-75, SURFACE STRENGTH OF PAPER (WAX PICK TEST)

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		H79	J51	MAJOR	MINOR	R.SDR	VAR			
L243	6	8.40	8.60	-0.95	.94	1.18	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L173A	6	8.40	7.20	-2.17	.24	1.07	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L230	6	9.00	9.20	-.13	.72	.92	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L122	6	9.00	8.20	-1.00	.22	1.21	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L366	6	9.20	9.80	.49	.35	.96	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L339	6	9.20	8.00	-1.07	-.05	1.25	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L195	6	9.20	9.20	-.03	.55	.96	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L183	6	9.80	9.00	.09	-.07	.47	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L228	6	10.00	7.00	-1.54	-1.24	.00	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L225	6	10.00	9.40	.54	-.04	1.34	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L182W	6	10.20	8.60	-.05	-.61	1.75	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L213	6	10.20	10.00	1.16	-.09	.47	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L236	6	10.20	9.40	.64	-.21	1.07	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L285	6	10.20	9.40	.64	-.21	1.75	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L378	6	10.40	10.80	1.95	.31	1.43	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L115	6	10.40	9.40	.74	-.39	1.18	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L162	6	11.00	9.00	.69	-1.11	.00	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
L616	#	11.20	13.60	4.78	1.02	1.67	50W	SURFACE PICK STRENGTH, WAX (TAPPI T459 6875)		
GMEANS:		9.69	8.95			1.00				
		95% ELLIPSE:		2.95	1.72	WITH GAMMA = 59 DEGREES				


SURFACE PICK STRENGTH, WAX.

SAMPLE H79 = 9.7

WAX NUMBER

SAMPLE J51 = 9.0

WAX NUMBER

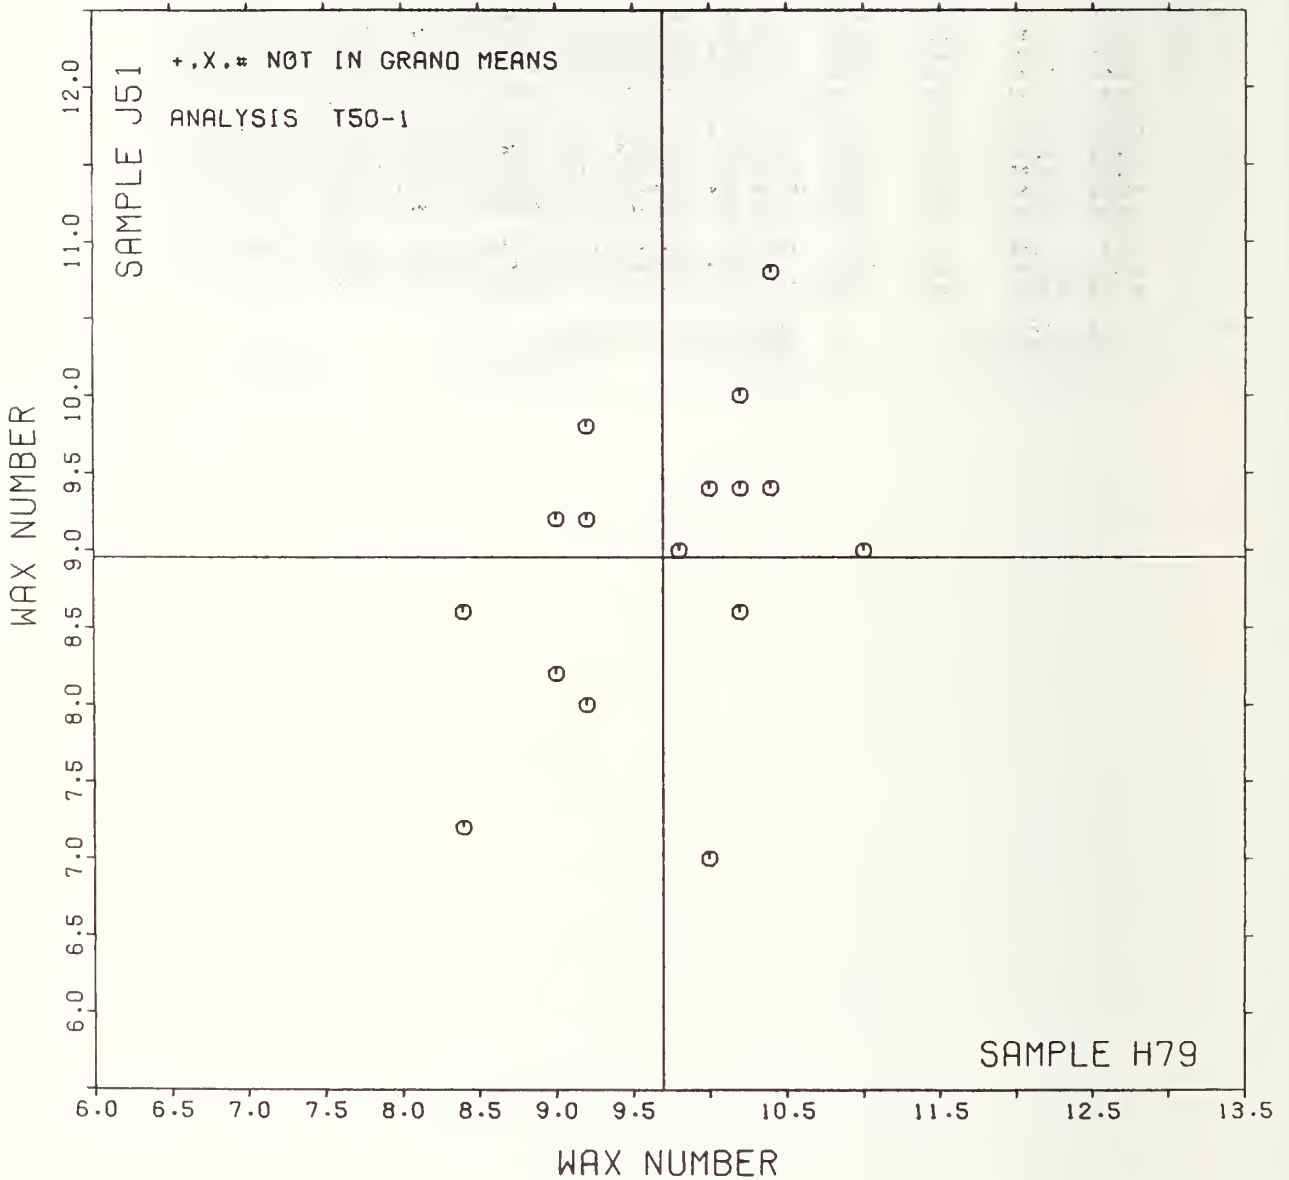

TAPPI COLLABORATIVE REFERENCE PROGRAM
ANALYSIS T91-1 TABLE 1
CONEORA (CORRUGATING MEDIUM TEST-CMT)
TAPPI STANDARD T809 6S-71

LAB CODE	LINERBOARD					KRAFT					TEST D. = 10		
	E72 MEAN	127 GRAMS PER SQUARE METER DEV	N. DEV	SDR	R. SDR	E83 MEAN	126 GRAMS PER SQUARE METER DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L176	235.	10.	.62	19.	1.47	306.	6.	.20	16.	.92	91P	0	L176
L182	234.	9.	.54	16.	1.25	321.	21.	.68	8.	.45	91N	0	L182
L185	243.	17.	1.10	15.	1.17	344.	45.	1.42	12.	.69	91A	0	L185
L218	290.	-35.	-2.23	11.	.82	278.	-21.	-.67	16.	.91	91A	0	L218
L242	240.	15.	.95	9.	.66	345.	46.	1.46	11.	.65	91G	0	L242
L255	213.	-12.	-.77	9.	.72	237.	-63.	-1.98	6.	.33	91P	0	L255
L269	215.	-10.	-.63	8.	.60	302.	3.	.09	14.	.82	91P	0	L269
L280	226.	1.	.07	14.	1.06	312.	13.	.40	26.	1.46	91N	0	L280
L289	237.	12.	.74	13.	1.02	248.	-52.	-1.63	30.	1.72	91P	0	L289
L329	212.	-13.	-.83	15.	1.15	301.	1.	.04	36.	2.02	91P	0	L329
L393	212.	-13.	-.83	14.	1.06	178.	-121.	-3.84	8.	.46	91P	#	L393
L394	215.	-11.	-.66	10.	.78	281.	-19.	-.59	15.	.86	91P	0	L394
L484	223.	-2.	-.14	6.	.48	305.	6.	.18	14.	.81	91N	0	L484
L621	211.	-14.	-.89	19.	1.42	274.	-25.	-.79	21.	1.19	91P	0	L621
L622	244.	19.	1.18	18.	1.38	305.	5.	.17	29.	1.63	91P	0	L622
L650	249.	23.	1.46	12.	.88	343.	44.	1.40	14.	.80	91N	0	L650
L665	218.	-8.	-.49	15.	1.14	288.	-12.	-.37	13.	.73	91P	0	L665

GR. MEAN = 225. NEWTONS
SD MEANS = 16. NEWTONS
AVERAGE SDR = 13. NEWTONS
GR. MEAN = 50.67 POUNDS
TOTAL NUMBER OF LABORATORIES REPORTING = 17

GRAND MEAN = 299. NEWTONS
SD OF MEANS = 32. NEWTONS
AVERAGE SDR = 18. NEWTONS
GRAND MEAN = 67.29 POUNDS

TEST DETERMINATIONS = 10
16 LABS IN GRAND MEANS

Best values: E72 225 + 20 newtons
E83 300 + 50 newtons

The following laboratories were omitted from the grand means because of extreme test results: 393


TAPPI COLLABORATIVE REFERENCE PROGRAM
ANALYSIS T91-1 TABLE 2
CONEORA (CORRUGATING MEDIUM TEST-CMT)
TAPPI STANDARD T809 6S-71

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY	TEST INSTRUMENT	CONDITIONS
		E72	E83	MAJOR	MINOR	R. SDR	VAR			
L218	0	190.	276.	-32.	27.	.86	91A	FLAT CRUSH STRENGTH,	CONEORA,	INSTRON
L501	0	211.	274.	-28.	5.	1.31	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L393	#	212.	178.	-119.	-27.	.76	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L329	0	212.	301.	-3.	13.	1.59	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L255	0	213.	237.	-63.	-9.	.53	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L394	0	215.	281.	-21.	4.	.82	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L269	0	215.	302.	-1.	10.	.71	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L665	0	218.	288.	-13.	4.	.93	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L484	0	223.	305.	5.	4.	.64	91N	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L280	0	226.	312.	12.	3.	1.26	91N	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L182	0	234.	321.	23.	-1.	.85	91N	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L176	0	235.	306.	9.	-7.	1.20	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L289	0	237.	248.	-45.	-28.	1.37	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L242	0	240.	345.	49.	1.	.65	91G	FLAT CRUSH STRENGTH,	CONEORA,	GAYDON PLAT CRUSH TESTER
L185	0	243.	344.	48.	-2.	.93	91A	FLAT CRUSH STRENGTH,	CONEORA,	INSTRON
L622	0	244.	305.	11.	-16.	1.50	91P	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
L650	0	249.	343.	49.	-8.	.84	91N	FLAT CRUSH STRENGTH,	CONEORA,	TMI/HINDE & DAUCH
GMEANS:		225.	299.			1.00				
		95% ELLIPSE:		54.	35.	WITH GAMMA = 70 DEGREES				

CONCORA (CMT)

SAMPLE E72 = 225. NEWTONS
 SAMPLE E72 = 50.7 POUNDS

SAMPLE E83 = 299. NEWTONS
 SAMPLE E83 = 67.3 POUNDS

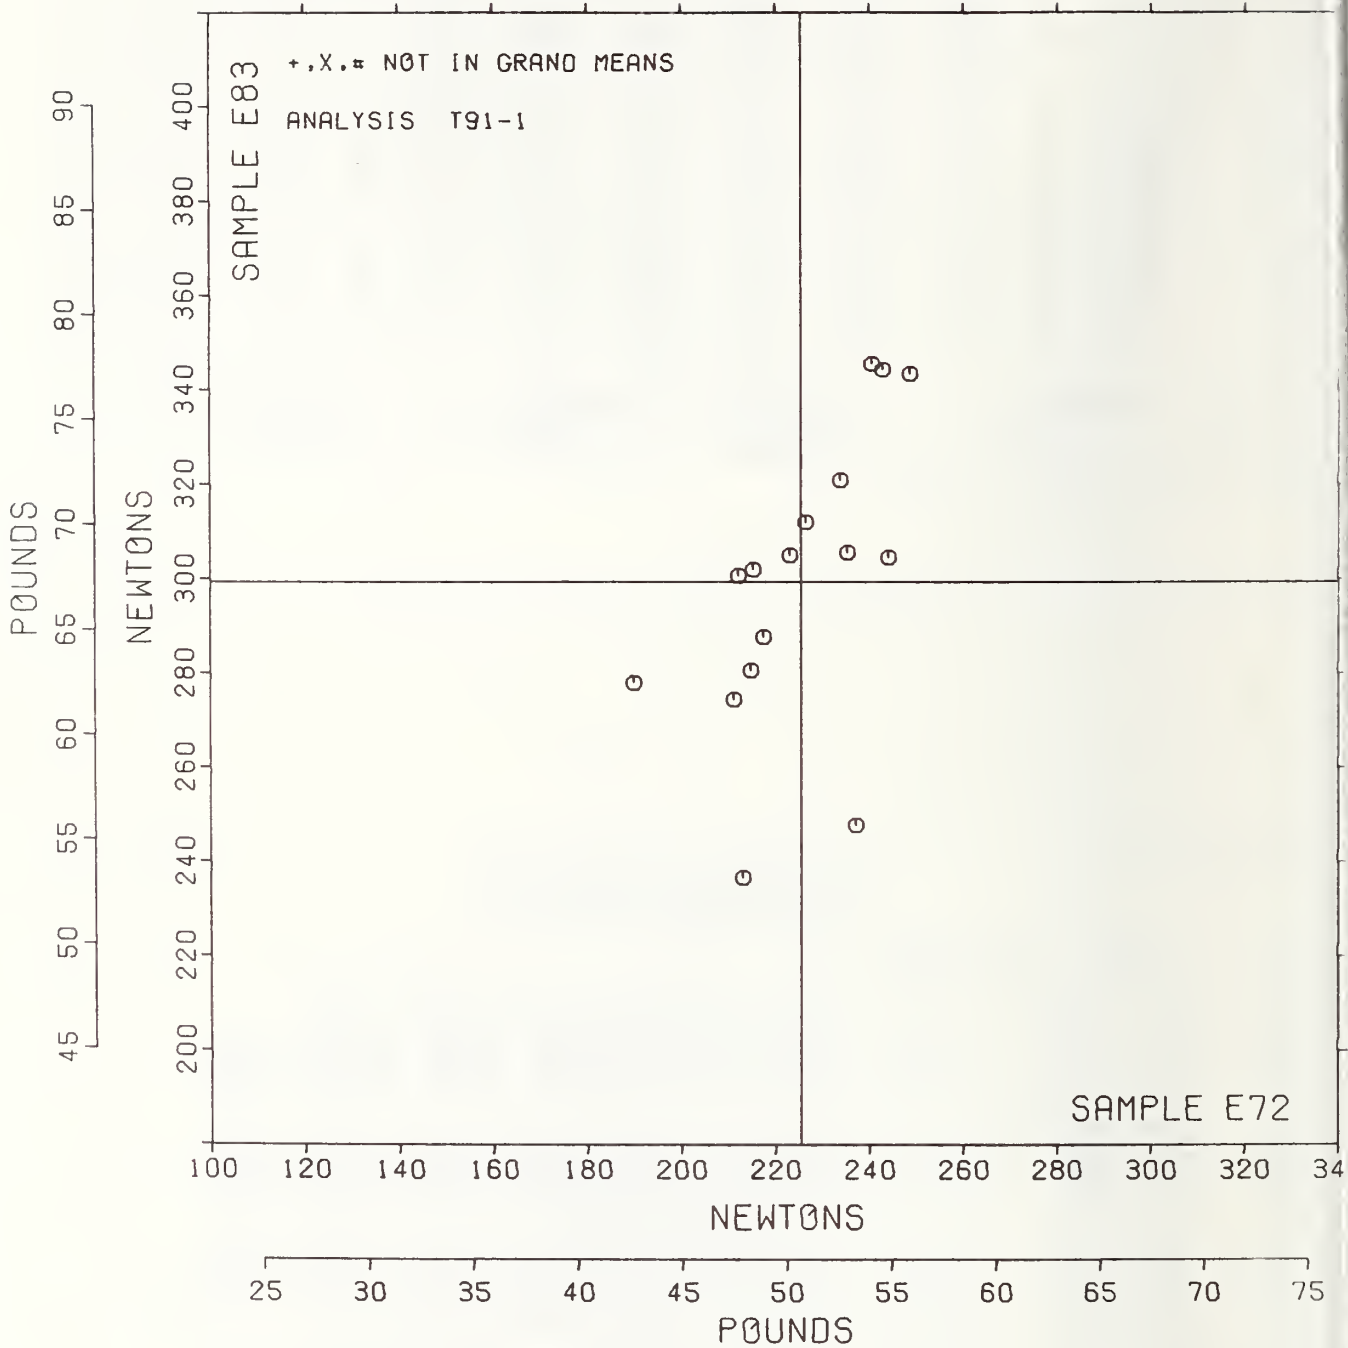


TAPPI COLLABORATIVE REFERENCE PROGRAM
 ANALYSIS T96-1 TABLE 2
 RING CRUSH (COMPRESSION RESISTANCE OF PAPERBOARD)
 TAPPI STANDARD T818 08-76

LAB CODE	F	MEANS		COORDINATES		AVG R.SDR VAR	PROPERTY==TEST INSTRUMENT==CONDITIONS
		E72	E83	MAJOR	MINOR		
L234	#	150.	100.	-70.	-19.	1.18 96P	RING CRUSH, TMI/HINDE & DAUCH
L621	0	161.	137.	-46.	9.	.78 96P	RING CRUSH, TMI/HINDE & DAUCH
L176	0	170.	133.	-42.	1.	1.45 96P	RING CRUSH, TMI/HINDE & DAUCH
L124	0	174.	141.	-34.	6.	1.68 96P	RING CRUSH, TMI/HINDE & DAUCH
L114	0	174.	137.	-35.	2.	1.20 96P	RING CRUSH, TMI/HINDE & DAUCH
L617	0	178.	126.	-38.	-9.	1.48 96I	RING CRUSH, INSTRON
L333	0	178.	136.	-33.	-1.	.60 96I	RING CRUSH, INSTRON
L237	0	180.	145.	-26.	6.	.79 96P	RING CRUSH, TMI/HINDE & DAUCH
L484	0	188.	152.	-16.	8.	.93 96R	RING CRUSH, REGMED
L336	0	198.	134.	-25.	-8.	.81 96P	RING CRUSH, TMI/HINDE & DAUCH
L570	0	195.	134.	-20.	-12.	.50 96P	RING CRUSH, TMI/HINDE & DAUCH
L126	0	196.	150.	-10.	1.	1.08 96P	RING CRUSH, TMI/HINDE & DAUCH
L663	0	197.	152.	-8.	2.	.92 96P	RING CRUSH, TMI/HINDE & DAUCH
L191	0	201.	153.	-4.	2.	2.47 96P	RING CRUSH, TMI/HINDE & DAUCH
L122	0	201.	145.	-8.	-5.	.83 96P	RING CRUSH, TMI/HINDE & DAUCH
L320	0	203.	154.	-2.	1.	.65 96P	RING CRUSH, TMI/HINDE & DAUCH
L350	0	218.	165.	16.	3.	.78 96P	RING CRUSH, TMI/HINDE & DAUCH
L141	0	218.	169.	19.	6.	.72 96P	RING CRUSH, TMI/HINDE & DAUCH
L305	*	219.	144.	6.	-16.	.64 96P	RING CRUSH, TMI/HINDE & DAUCH
L182	0	220.	161.	17.	-2.	.71 96N	RING CRUSH, TMI/HINDE & DAUCH
L303	0	225.	166.	23.	-0.	.74 96N	RING CRUSH, TMI/HINDE & DAUCH
L649	0	225.	161.	21.	-4.	.68 96P	RING CRUSH, TMI/HINDE & DAUCH
L610	0	226.	173.	27.	4.	.87 96P	RING CRUSH, TMI/HINDE & DAUCH
L553	0	229.	175.	31.	5.	1.43 96P	RING CRUSH, TMI/HINDE & DAUCH
L623	0	236.	178.	39.	3.	.78 96P	RING CRUSH, TMI/HINDE & DAUCH
L650	0	237.	172.	36.	-1.	.66 96N	RING CRUSH, TMI/HINDE & DAUCH
L603	0	246.	185.	51.	4.	1.05 96P	RING CRUSH, TMI/HINDE & DAUCH
L242	0	260.	183.	62.	-5.	1.41 96G	RING CRUSH, GAYDON FLAT CRUSH TESTER
L1C7	#	367.	346.	240.	76.	3.40 96P	RING CRUSH, TMI/HINDE & DAUCH
MEANS:		205.	154.			1.00	
		95% ELLIPSE:		80.	16.	WITH GAMMA = 32 DEGREES	

RING CRUSH

SAMPLE E72 = 205. NEWTONS
 SAMPLE E72 = 46.1 POUNDS

SAMPLE E83 = 154. NEWTONS
 SAMPLE E83 = 34.7 POUNDS

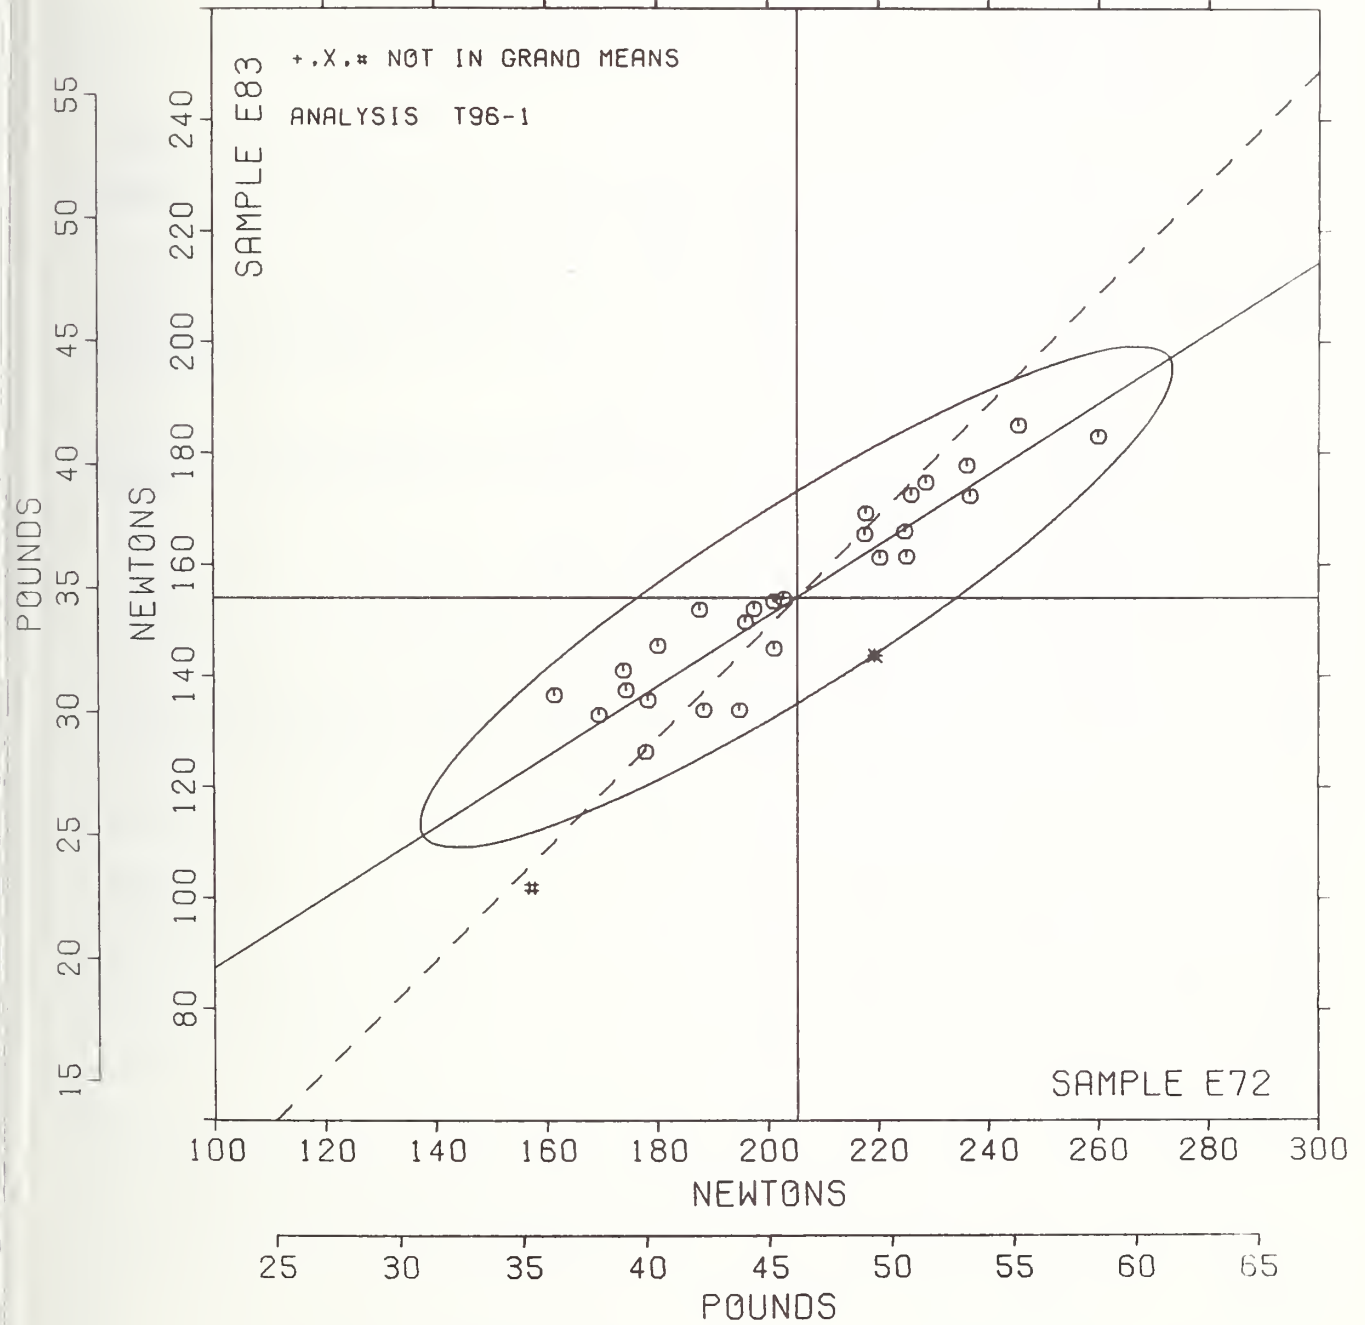

SUMMARY TABLE

TEST METHOD	SAMPLE CODE	GRAND MEAN	SD OF MEAN	AVER SDR	REPL CRP	LABS INCL	LABS PARTIC	REPL TAPPI	REPEAT	REPROD
BURSTING STRENGTH, MODEL C T10=1 PSI	H63	16.69	1.32	1.04	15	42	47	10	.91	3.70
	J39	28.89	2.11	1.48					1.30	5.88
BURSTING STRENGTH, MODEL C=A T10=2 PSI	H63	16.66	1.62	1.14	15	31	32	10	1.00	4.53
	J39	28.70	1.93	1.47					1.29	5.40
BURSTING STRENGTH, HIGH RANGE T11=1 PSI	E77	74.6	3.3	5.0	15	35	45	10	4.4	9.4
	K29	59.4	2.5	4.1					3.6	7.1
TEARING STRENGTH, DEEP CUTOUT T15=1 GRAMS	E76	85.9	3.8	2.5	15	115	125	10	2.2	10.7
	E80	57.6	3.7	1.5					1.3	10.2
TEARING STRENGTH, NO CUTOUT T17=1 GRAMS	J41	67.2	3.3	2.8	15	11	12	10	2.5	9.4
	K19	151.5	10.3	8.0					7.0	28.9
TENSILE STRENGTH, PACKAGING PAPERS T19=1 KILONEWTN/M	J15	8.58	.33	.32	20	45	48	12	.25	.93
	K31	8.58	.30	.45					.36	.87
TENSILE STRENGTH, CRE TYPE T20=1 KILONEWTN/M	J04	3.67	.18	.17	20	41	49	12	.14	.50
	J08	6.09	.30	.37					.30	.84
TENSILE STRENGTH, PENDULUM TYPE T20=2 KILONEWTN/M	J04	3.75	.21	.21	20	33	35	12	.17	.59
	J08	6.22	.40	.43					.34	1.12
T.E.A., PACKAGING PAPERS T25=1 JOULES/SQ M	J15	121.6	11.3	12.5	20	15	16	12	10.0	32.1
	K31	76.1	8.0	10.1					8.1	22.7
T.E.A., PRINTING PAPERS T26=1 JOULES/SQ M	J04	37.7	2.6	4.1	20	14	15	12	3.2	7.4
	J08	75.8	6.6	7.4					5.0	18.8
ELONGATION TO BREAK, PACKAGING PAPER T28=1 PERCENT	J15	2.118	.080	.145	20	14	18	12	.116	.232
	K31	1.457	.076	.110					.088	.218
ELONGATION TO BREAK, PRINTING PAPER T29=1 PERCENT	J04	1.540	.201	.119	20	17	20	12	.095	.560
	J08	1.842	.182	.150					.120	.510
FOLDING ENDURANCE (MIT) T30=1 DOUBLE FOLDS	J29	24.3	7.0	9.3	15	44	50	10	8.2	19.9
	J31	72.9	15.1	17.9					15.7	42.7
FOLDING ENDURANCE (MIT) T30=2 LOG(10) FOLD	J29	1.342	.112	.155	15	45	50	10	.136	.319
	J31	1.839	.097	.117					.103	.274
STIFFNESS, GURLEY T35=1 GURLEY UNITS	H69	452.	28.	21.	10	30	32	10	18.	77.
	J25	242.	17.	13.					12.	46.
STIFFNESS, TABER T36=1 TABER UNITS	J10	16.52	1.02	.76	10	25	29	5	.94	2.90
	J69	5.96	1.02	.35					.43	2.85
SURFACE PICK STRENGTH, IGT T49=1 KP CM/SEC	H79	86.7	51.5	5.0	4	11	16	4	6.9	142.5
	E60	75.5	49.0	4.9					6.7	135.7
SURFACE PICK STRENGTH, WAX T50=1 WAX NUMBER	H79	9.69	.75	.48	5	17	18	5	.59	2.07
	J51	8.95	.96	.45					.56	2.66
CONCRETE (CMT) T91=1 NEWTONS	B72	225.	16.	13.	10	16	17	10	11.	44.
	B83	299.	32.	18.					15.	88.
RING CRUSH T96=1 NEWTONS	E72	205.	26.	13.	10	27	29	10	11.	71.
	E83	154.	17.	10.					9.	47.

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. TAPPI CRP 55S	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE Technical Association of the Pulp and Paper Industry COLLABORATIVE REFERENCE PROGRAM FOR PAPER Report #55S		5. Publication Date January 10, 1978	6. Performing Organization Code
7. AUTHOR(S) R. G. Powell, J. Horlick	8. Performing Organ. Report No. NBSIR 79-1358		
9. PERFORMING ORGANIZATION NAME AND ADDRESS NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, DC 20234		10. Project/Task/Work Unit No.	11. Contract/Grant No.
12. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS (Street, City, State, ZIP) Collaborative Testing Services, Inc., 9241 Wood Glade Drive, Great Falls, Virginia 22066; and Technical Association of the Pulp and Paper Industry		13. Type of Report & Period Covered Final	14. Sponsoring Agency Code
15. SUPPLEMENTARY NOTES <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.			
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.) Collaborative Reference Programs provide participating laboratories with the means for checking periodically the level and uniformity of their testing in comparison with that of other participating laboratories. An important by-product of the programs is the provision of realistic pictures of the state of the testing art. This is one of the periodic reports showing averages for each participant, within and between laboratory variability, and other information for participants and standards committees.			
17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons) Collaborative reference program; Laboratory evaluation; Paper; Precision; Reference samples, Testing calibration			
18. AVAILABILITY <input type="checkbox"/> Unlimited <input checked="" type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office, Washington, DC 20402, SD Stock No. SN003-003- <input type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA, 22161	19. SECURITY CLASS (THIS REPORT) UNCLASSIFIED	21. NO. OF PRINTED PAGES 69	
20. SECURITY CLASS (THIS PAGE) UNCLASSIFIED		22. Price	



This diagram is composed of two full-size overlaid tracings. One tracing was made from the Thwing-Elmendorf tear tester with NO CUTOUT (old style). The other tracing was made from the Thwing-Elmendorf tear tester with DEEP CUTOUT. The cross hatched area represents the metal removed from the swinging sector when the deep cutout (new) style was created.

DEEP CUTOUT instrument
is $\frac{5}{8}$ inch across

NO CUTOUT instrument
is $1 \frac{1}{4}$ inch across

Note shape of pendulum
sector with respect to
an imaginary line drawn
across the top of the
specimen clamp

